



Standard Test Method for Transverse Rupture Strength of Metal Powder Specimens¹

This standard is issued under the fixed designation B 528; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method covers determination of the transverse rupture strength of sintered, including post-treated, metal powder test specimens by subjecting them to a uniformly increasing transverse force under controlled conditions. The term “transverse rupture strength” as used herein, defines the stress, calculated from the flexure formula required to break a specimen as a simple beam supported near the ends and applying the force midway between the fixed line center of the supports.

1.2 *Limitations*—The transverse rupture test is only applicable to relatively brittle materials. In cases where a ductile specimen is being tested and the permanent deflection as a result of testing exceeds 0.020 in. (0.50 mm), the test results may be questionable.

1.3 Test Method B 406 should be consulted for determining the transverse rupture strength of cemented carbides.

1.4 The values stated in inch-pound units are to be regarded as the standard. The SI values are provided for information only.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards*:²

B 243 Terminology of Powder Metallurgy

B 312 Test Method for Green Strength for Compacted Metal Powder Specimens

B 406 Test Method for Transverse Rupture Strength of Cemented Carbides

B 925 Practices for Production and Preparation of Powder Metallurgy (P/M) Test Specimens

3. Terminology

3.1 *Definitions*—For definitions of terms in this test method, see Terminology B 243.

4. Significance and Use

4.1 This test method is used to measure the strength of sintered, including post-treated, specimens. Transverse rupture strength is not a design value. For many sintered materials, transverse rupture strength is approximately twice the ultimate tensile strength.

5. Apparatus

5.1 *Micrometer*, capable of measuring with a resolution of 0.0001 in. (0.002 mm).

5.2 *Transverse Rupture Strength Fixture*, as shown in Fig. 1.

5.3 *Compression Testing Machine*, capable of applying a breaking force on the test specimen with an accuracy of 1.0 % and readable to the nearest 10 lbf (50 N).

6. Test Specimen

6.1 The thin test specimen shall have the shape and dimensions shown in the figure titled P/M Transverse Rupture Strength Test Specimen of Practices B 925.


7. Procedure

7.1 Prepare test specimens by pressing and sintering using tooling shown in the figure titled Transverse Rupture Test Specimen, Typical Laboratory Tooling of Practices B 925, or machine from finished parts. Measure the width and thickness of the specimens to the nearest 0.001 in. (0.03 mm) with a micrometer.

¹ This test method is under the jurisdiction of ASTM Committee B09 on Metal Powders and Metal Powder Products and is the direct responsibility of Subcommittee B09.05 on Structural Parts.

Current edition approved Nov. 1, 2005. Published November 2005. Originally approved in 1970. Last previous edition approved in 1999 as B 528 – 99.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

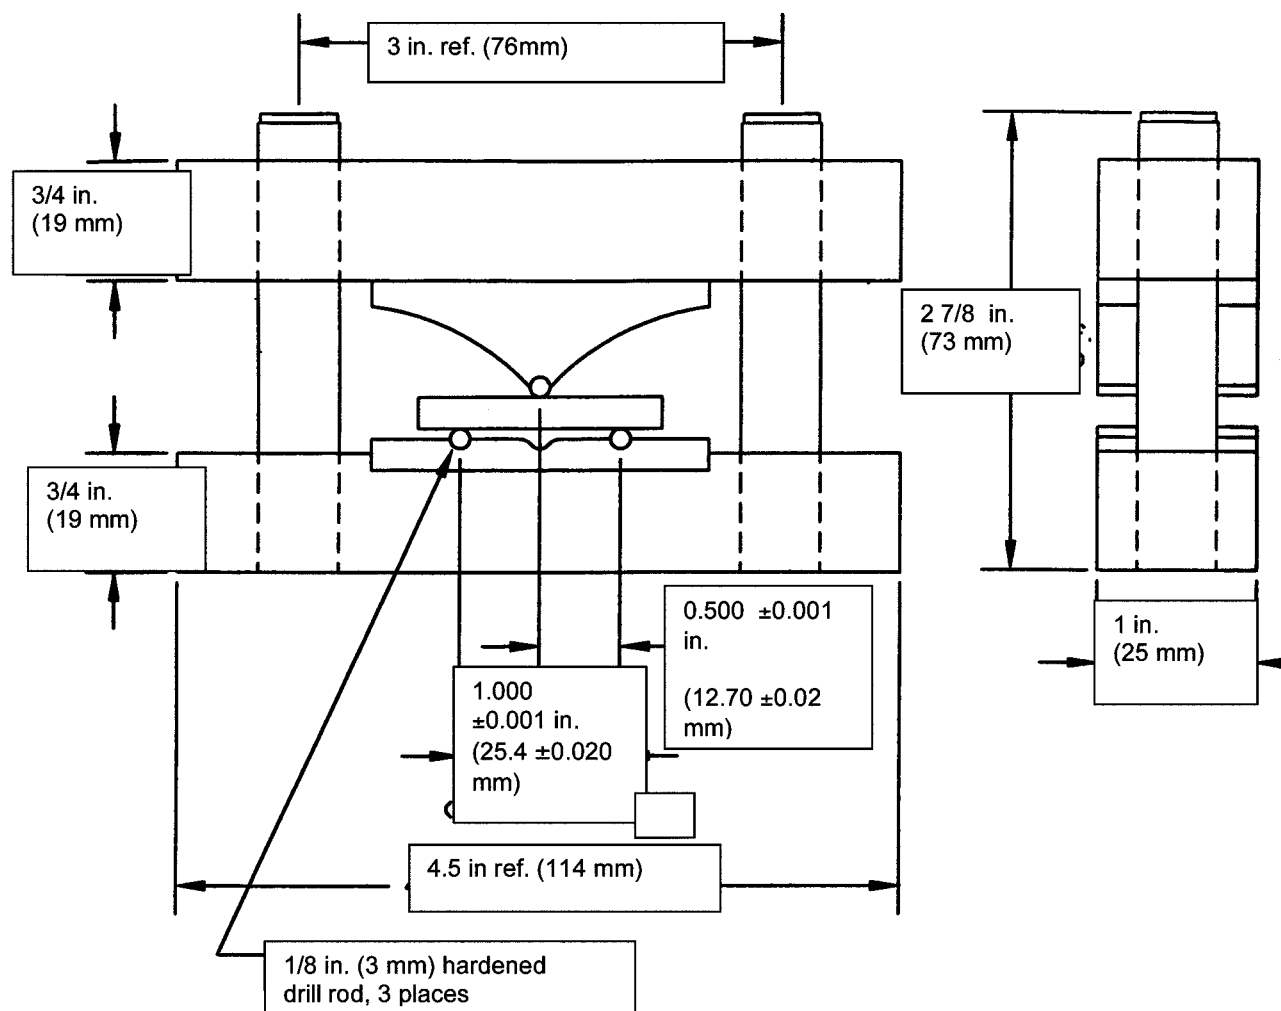

NOTE—This fixture is used in Test Method B 312.

FIG. 1 Transverse Rupture Test Fixture

7.2 Locate the specimen in the transverse rupture test fixture perpendicular to the supporting rods. Apply compressive force parallel to the pressing direction of the specimen at a no-load crosshead speed of not greater than 0.2 in. (5.0 mm)/min until rupture occurs. Record this breaking force to the nearest 10 lbf (50 N).

8. Calculation

8.1 Calculate the transverse rupture strength of the specimen as follows:

$$TRS = (3 \times P \times L) / (2 \times t^2 \times w) \quad (1)$$

where:

TRS = transverse rupture strength of the specimen, psi (MPa),

P = force required to rupture the specimen, lbf (N),

L = length of specimen span relative to fixture 1.000 in. (25.4 mm),

w = width of the specimen, in. (mm), and

t = thickness of specimen, in. (mm).

9. Report

9.1 Report the transverse rupture strength in pounds-force per square inch (megapascals) to the nearest 1000 psi (10 MPa). When reporting the results, state the following supplementary data to clarify the results:

9.1.1 Identification of the material being tested, that is, composition, density, state of heat treatment, and compacted or machined specimen.

10. Precision

10.1 On the basis of test error alone, the difference in the absolute value of two test results, x_1 and x_2 , obtained in the same laboratory on the same material, will be expected to exceed r , (the repeatability interval) only about 5 % of the time. If such a difference is found to be larger than r there is reason to question one or both results. The value of r varies proportionally with the magnitude of the transverse rupture strength and is calculated from the following equation:

$$r = 6700 + (0.064)(x - 41000) \quad (2)$$

where the units of r and x are psi. This applies over the range from x from 41 500 to 145 000 psi. The unit x is the average of the two points being checked.

$$\frac{x_1 + x_2}{2} = x \quad (3)$$

10.2 On the basis of test error alone, the difference in absolute value of two test results, x_1 and x_2 , obtained in different laboratories on the same material, will be expected to exceed R , the reproducibility interval, only about 5 % of the time. If such a difference is found to be larger than R there is reason to question one or both results. The value of R varies proportionally with the magnitude of the transverse rupture strength and is calculated from the following equation:

$$R = 8900 + (0.122) (x - 41000) \quad (4)$$

where units of R and x are psi.

10.3 The value of r and R are assumed to vary linearly over the transverse rupture strength range from 41 500 to 145 000 psi. Transverse rupture strength was measured only at the two end points.

11. Keywords

11.1 flexural strength; 3 Point Bend Test; transverse rupture; transverse rupture strength; TRS

SUMMARY OF CHANGES

Committee B09 has identified the location of selected changes to this standard since the last issue, B 528 – 99, that may impact the use of this standard. (Approved Nov. 1, 2005.)

- (1) Added Summary of Changes.
- (2) Added Practices B 925 to Referenced Documents.
- (3) Deleted 5.1, 5.2, and 5.3 and renumbered subsequent sections.
- (4) In 6.1, added reference to figure in Practices B 925 for specimen shape.
- (5) In 7.1, added reference to figure in Practices B 925 for tools to press a test specimen.
- (6) Deleted old Fig. 1 for tooling to press the compact and replaced it with reference to Practices B 925.
- (7) Renumbered old Fig. 2 as Fig. 1 and changed the dimensions on the test fixture to conform with modern drawing practices.
- (8) Deleted old Fig. 3 which shows the shape and dimensions of the test specimen, and replaced it with a reference to the specimen shape in Practices B 925.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).