



Standard Test Method for Absorption Coefficient of Ethylene Polymer Material Pigmented with Carbon Black¹

This standard is issued under the fixed designation D3349; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method measures the amount of light transmitted through a film of carbon black pigmented ethylene polymer.

1.2 After calculation of the amount of light and film thickness, an absorption coefficient is calculated.

1.3 Whenever two sets of values are presented, in different units, the values in the first set are the standard, while those in parentheses are for information only.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

E60 Practice for Analysis of Metals, Ores, and Related Materials by Spectrophotometry

D1248 Specification for Polyethylene Plastics Extrusion Materials for Wire and Cable

3. Summary of Test Method

3.1 The transmission of light of a specified wavelength through thin ethylene polymer film is measured. The result is used to calculate an absorption coefficient that is a reciprocal function of transmission after correction for thickness.

4. Significance and Use

4.1 The absorption coefficient of polyolefin polymer pigmented with carbon black is useful to judge the degree and uniformity of dispersion of the pigment, and the adequacy of the quantitative level of pigment addition. These factors are

used to predict the performance of the polymer material in response to prolonged exposure to ultraviolet light as evidenced by minimal changes in specific properties.

NOTE 1—This test method was developed to evaluate ethylene polymer materials pigmented with small particle size carbon blacks suitable for UV protection. It is not known how accurate and reproducible the test would be with larger (35 nm or greater) particle size blacks.

5. Apparatus

5.1 *Spectrophotometer*—An instrument in accordance with Practice **E60** is required.

NOTE 2—Consult the spectrophotometer's operation manual or consult the manufacturer of the instrument for the calibration procedure.

5.2 *Mold*—A mold in accordance with **Figs. 1 and 2**. Make the mold of Ketos steel (or equivalent) hardened to Rockwell C45, with mold surfaces chromium plated to 0.005-mm (0.0002-in.) minimum thickness.

5.3 *Specimen Holder*—Cut two concentric rings from phenolic-paper laminate or other suitable material to the dimensions shown in **Fig. 3**. Slip fit the rings snugly one within the other.

5.4 *Reference Material*—A reference material is required having an absorbance value of 1.0 to 1.2 at 375 nm as measured by the instrument used for testing.

5.4.1 *Neutral Density Filter*,³ M-type carbon 0.85 density, laminated between cellulose acetate sheets has been found satisfactory. Since this material is furnished as a rigid sheet, it cannot be mounted as described in Section 7. Instead, a special mount must be prepared by cutting Ring 1 of **Fig. 3** in half around its circumference to give two rings about 2 mm (0.08 in.) thick. Cut a 22-mm (0.87-in.) circle from the laminated filter, sandwich this between the two 2-mm rings, and slide the outer ring (Ring 2 of **Fig. 3**) over this composite.

5.4.2 An alternative reference material can be prepared by any user of this test method. Prepare an alternative reference material consisting of a highly uniform sample of ASTM Type I polyethylene (see Specification **D1248**) containing about 1 %

¹ This test method is under the jurisdiction of ASTM Committee D09 on Electrical and Electronic Insulating Materials and is the direct responsibility of Subcommittee D09.18 on Solid Insulations, Non-Metallic Shieldings and Coverings for Electrical and Telecommunication Wires and Cables.

Current edition approved Jan. 1, 2012. Published February 2012. Originally approved in 1974. Last previous edition approved in 2006 as D3349 – 06. DOI: 10.1520/D3349-12.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The sole source of supply of the apparatus known to the committee at this time is The Kodak neutral density filter, No. 5, available from the Eastman Kodak Co.. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

*A Summary of Changes section appears at the end of this standard.



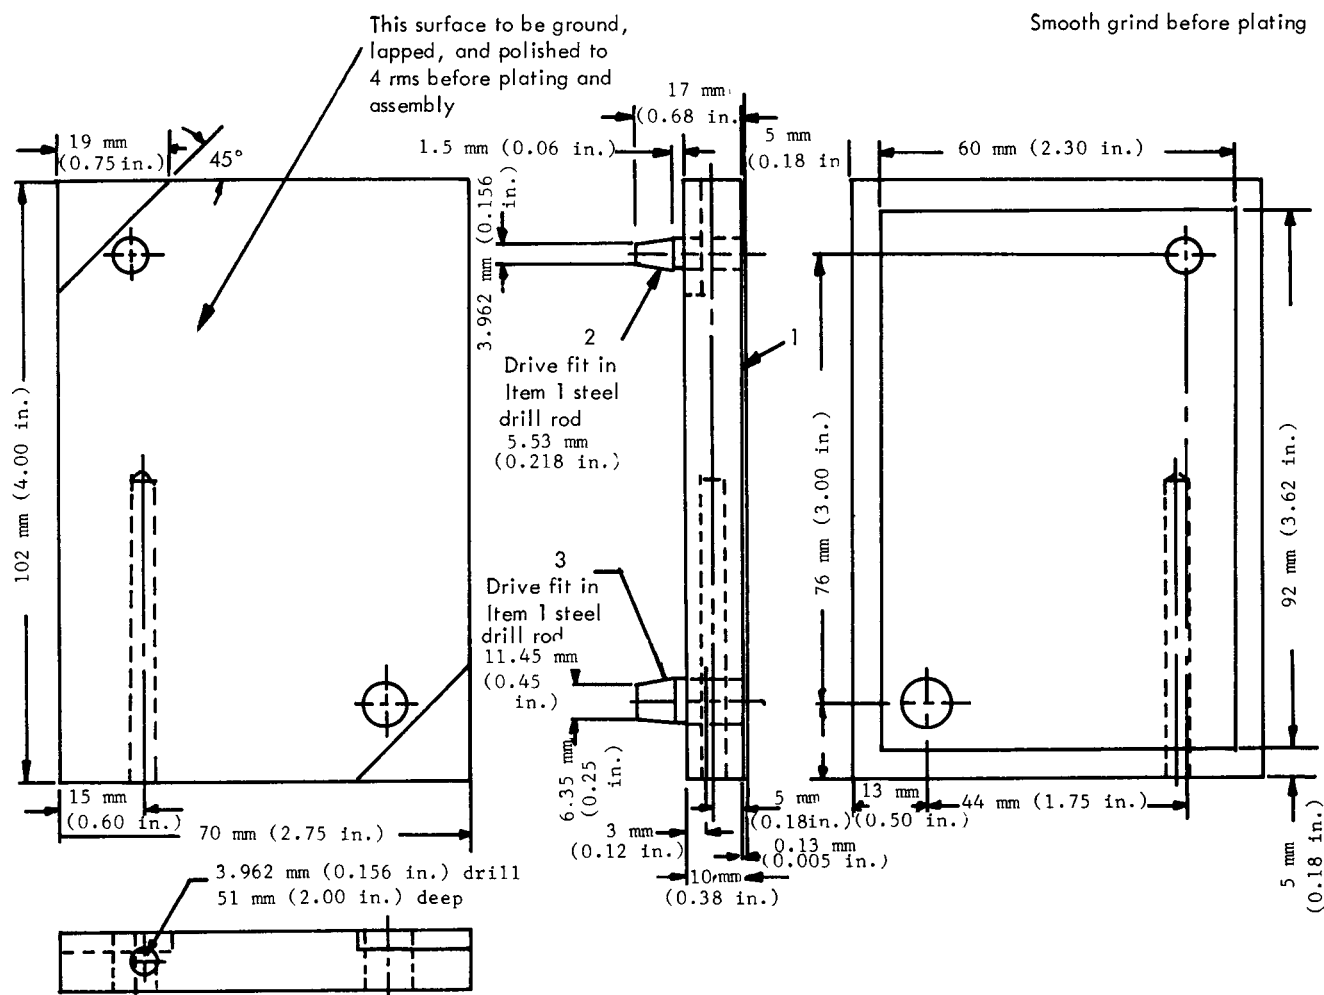


FIG. 2 Mold, Bottom Platen

9.2 Close the shutter and recheck the reference material. Rotate the specimen to bring the next 120° mark to the top and obtain the absorbance value v_2 . Repeat the procedure with the third 120° mark at the top to obtain the value v_3 . Average the values v_1 , v_2 , and v_3 to obtain the average absorbance $\bar{v}$. If any value of v differs from $\bar{v}$ by more than 10 %, discard the specimen and replace it.

9.3 Remove the film from the specimen mounting rings by cutting it carefully along the boundary between the two rings and weigh it to the nearest 0.0001 g. The No. 11 Bard-Parker scalpel blade⁴ in a suitable handle has been found very effective for the cutting operation. Measure the diameter and calculate the area of the specimen. Calculate average specimen thickness as follows:

$$t = (10^{-2} \cdot W) / (D \cdot A) \quad (1)$$

⁴ The sole source of supply of the apparatus known to the committee at this time is the No. 11 Bard-Parker scalpel blade, available from most laboratory supply houses. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

where:

t = thickness, m,
 W = weight, g,
 D = density, g/cm³, and
 A = area, cm².

NOTE 3—The nominal density value for black low density ethylene polymer is 0.932 g/cm³.

9.4 Repeat 9.1-9.3 for the second and third specimens.

10. Calculation


10.1 Calculate the absorption coefficient of each specimen, in turn, as follows:

$$a = (10^{-3} \cdot 2.303 \cdot \bar{v}) / (t) \quad (2)$$

where:

a = absorption coefficient, 1000 (absorbance/metre), at 375 nm,
 $\bar{v}$ = average absorbance as found in 9.2, and
 t = thickness, m, as found in 9.3.

10.2 Average the three values, a , for the three specimens to obtain the value for the sample.

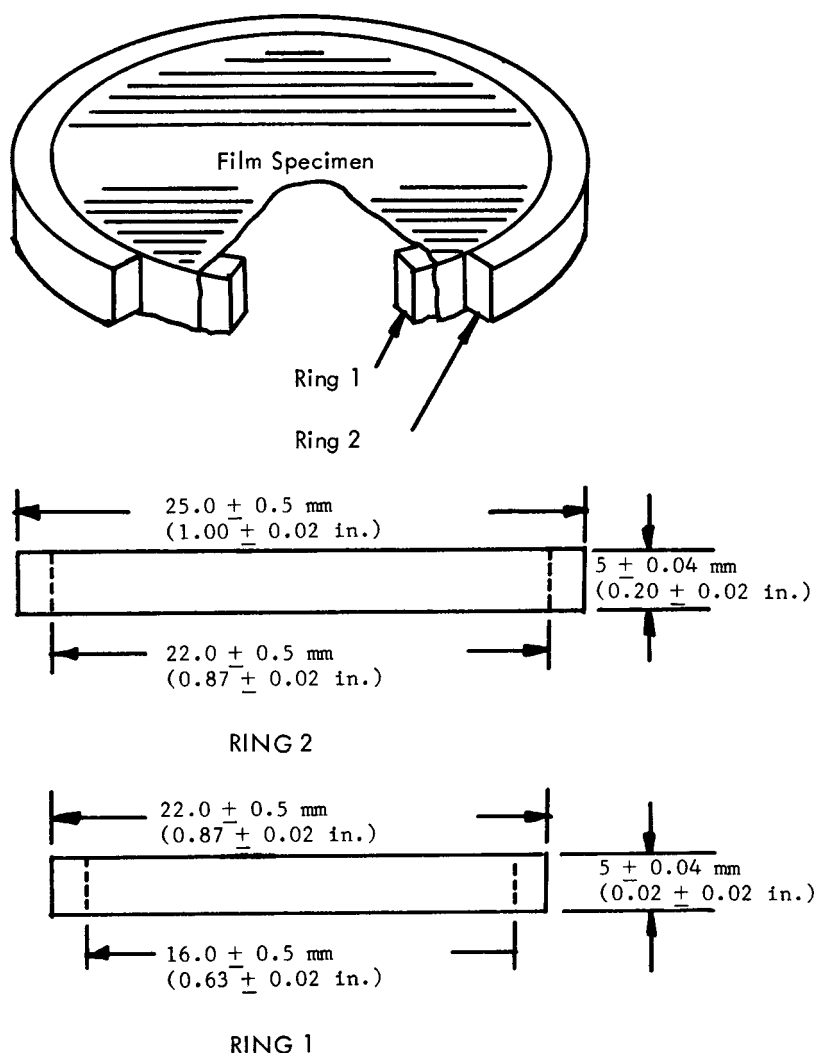

NOTE 1—If required, adjust either the inside diameter of Ring 2 or outside diameter of Ring 1 to obtain a snug fit of pressed film.

FIG. 3 Specimen Mounting Rings

11. Report

11.1 Report the following:

11.1.1 Complete identification of the material tested,

11.1.2 Nominal density of the material tested,

11.1.3 Calculated absorption coefficient of each specimen tested,

11.1.4 Average absorption coefficient of three specimens tested, which is the value for the sample, and

11.1.5 Type and model of spectrophotometer used.

11.1.6 Date of test

11.1.7 Name of operator

12. Precision and Bias

12.1 Precision:

12.1.1 In the early 1970's, a round-robin study was conducted by five laboratories using one sample of carbon black-pigmented ethylene polymer and the same make and model of spectrophotometer. Each laboratory molded from two to five test specimens from the sample and determined the

absorption coefficient of each. The following statistics, each expressed in the units of 1000 (absorbance/metre), were derived from the data submitted for this one sample.

Mean = 443
 S_r = 24
 S_R = 43

12.1.2 Interpretation of the data for the intervals S_r and S_R given above are as follows.

12.1.2.1 *Repeatability*—In comparing two averages (of three specimens each) for the sample obtained in one laboratory by one operator on the same day, the averages are judged as not equivalent if they differ by more than S_r .

12.1.2.2 *Reproducibility*—In comparing two averages (of three specimens each) for the sample obtained in different laboratories by different operators on different days, the averages are judged as not equivalent if they differ by more than S_R .

12.1.2.3 The judgments in 12.1.2.1 and 12.1.2.2 will be correct in approximately 95 % of such comparisons.

12.2 Bias:

12.2.1 In the round-robin study, it was found that different makes and models of spectrophotometer can produce systematically different results for the average absorbance of a specimen, with the maximum consistent difference being 6 % relative for the four types of instrument used in the study.

12.2.2 In critical applications, such as conformance of a material to a specification, it is necessary for the buyer and seller to agree upon the instrument that is to be used or to establish a correlation between the two types of instruments in use.

13. Keywords

13.1 absorption coefficient; carbon black; ethylene polymer

SUMMARY OF CHANGES

Committee D09 has identified the location of selected changes to this test method since the last issue, D3349 – 06, that can impact the use of this test method. (Approved January 1, 2012)

(1) Corrected non-mandatory language and clarified **Note 1**.

(2) Changed note in **Fig. 3**.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).