



Standard Practice for Fabricating and Checking Aluminum Alloy Ultrasonic Standard Reference Blocks¹

This standard is issued under the fixed designation E127; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This specification has been approved for use by agencies of the Department of Defense.

1. Scope

1.1 This practice covers a procedure for fabricating aluminum alloy ultrasonic standard reference blocks that can be used for checking performance of ultrasonic testing equipment and for standardization and control of ultrasonic tests of aluminum alloy products using pulsed longitudinal waves introduced into test material either by the direct-contact method or by the immersion method. A recommended procedure for checking blocks is described and calibration data for a number of reference blocks are tabulated. Statements concerning procedures are provided without a discussion of the technical background for the preference. The necessary technical background can be found in Refs. (1-16).²

NOTE 1—Practice E428 and Guide E1158 also describe procedures for selecting material, fabricating blocks, and checking response. Unlike this practice, there is no requirement for evaluation relative to a specified standard target.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:³

E317 Practice for Evaluating Performance Characteristics of Ultrasonic Pulse-Echo Testing Instruments and Systems without the Use of Electronic Measurement Instruments

¹ This practice is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.06 on Ultrasonic Method.

Current edition approved Feb. 15, 2010. Published March 2010. Originally approved in 1958. Last previous edition approved in 2007 as E127 - 07. DOI: 10.1520/E0127-10.

² The boldface numbers in parentheses refer to the list of references at the end of this practice.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E428 Practice for Fabrication and Control of Metal, Other than Aluminum, Reference Blocks Used in Ultrasonic Testing

E1158 Guide for Material Selection and Fabrication of Reference Blocks for the Pulsed Longitudinal Wave Ultrasonic Testing of Metal and Metal Alloy Production Material

E1316 Terminology for Nondestructive Examinations

E1324 Guide for Measuring Some Electronic Characteristics of Ultrasonic Examination Instruments

3. Terminology

3.1 *Definitions*—For definitions of terms not specific to this practice, refer to Terminology E1316.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *angular error*—the condition observed in ultrasonic tests of reference blocks when the response from the hole bottom is not maximum while the search unit is positioned to obtain either a maximum number of back reflections from a reference block or a maximum indication from its entry surface. Angular error results when the entry surface, hole bottom, and back surface are not parallel to each other.

3.2.2 *area-amplitude response curve*—a curve showing the relationship between different areas of reflecting targets located at a constant distance in an ultrasonic transmitting medium and their respective amplitudes of ultrasonic response.

3.2.3 *back reflection*—the indication, observed on the display screen of a test instrument, that represents the ultrasonic energy reflected from the back surface of a reference block.

3.2.4 *back surface*—the end of a reference block that is opposite the entry surface.

3.2.5 *entry surface*—the end of a reference block through which ultrasonic energy must pass when reflections from the hole bottom are obtained.

3.2.6 *hole bottom*—the flat reflecting surface in a reference block that is obtained by making the entire end of a drilled hole smooth and flat using best machining practices. The hole bottom is parallel to the entry surface of the block.

3.2.7 *hole size*—the diameter of the hole in a reference block that determines the area of the hole bottom.

3.2.8 *metal distance*—the distance in a reference block from its entry surface to the hole bottom.

3.2.9 *reference block*—an aluminum block, containing as an artificial discontinuity a flat-bottom drilled hole of known size.

3.2.10 *ultrasonic response*—the height of the indication, observed on a display screen of a test instrument, that represents the amount of ultrasonic energy initially reflected from the hole bottom in a reference block. Units usually used in measuring height of indication are inches, trace-to-peak, or percent of upper linearity limit.

4. Summary of Practice

4.1 Aluminum alloy stock is ultrasonically evaluated to ensure freedom from significant discontinuities and is then precisely fabricated into cylindrical blocks of prescribed lengths. A single, flat-bottom hole of specific diameter is drilled to a constant depth into the end of each block at its center, and the blocks are grouped into sets according to hole size and block length, or metal distance.

4.2 Each block is checked ultrasonically using a calibrated ultrasonic test system at a prescribed test frequency. Distance-amplitude and area-amplitude characteristics are established for sets of fabricated blocks using specific reflectors to provide a standard response. Curves are plotted to establish the interrelationship between the various blocks in the sets.

4.3 To permit the use of instrumentation similar to that originally used in developing this practice, or types more recently manufactured, two alternative test system calibration procedures are described. The first method (ball-to-block) which utilizes steel balls as reference standards, is covered in 11.8.2. The second method (block-to-block), which requires as reference standards, blocks which have been calibrated by the National Institute of Standards and Technology (NIST), is described in Annex A1.⁴

5. Significance and Use

5.1 Reference blocks fabricated to this practice will exhibit specific area-amplitude and distance-amplitude relationships only with an immersion test at 5 MHz using the search unit, test instrument, and test parameters described in this practice. Comparison tests at other frequencies or with uncalibrated test systems will not necessarily give the same relationships shown in this practice.

NOTE 2—The 1964 and prior issues of this practice required a test frequency of 15 MHz. Blocks conforming to earlier issues of this practice may not produce ultrasonic responses that conform to this issue. See Section 13 regarding provision for recertification or correction curves and tables.

5.2 Although the primary ultrasonic evaluation of blocks is performed at a specified frequency, the blocks may be used to standardize ultrasonic tests at any frequency and with any pulse-echo ultrasonic test system. Establishment of distance-

TABLE 1 Dimensions and Identification of Reference Blocks in the Basic Set (see Fig. 1)

Block Identification Number	Hole Diameter (A)	Metal Distance (B)		Overall Length (C)	
	$\frac{1}{64}$ ths in.	in.	mm	in.	mm
3-0300	3	3.000	76.2	3.750	95.2
5-0012	5	0.125	3.2	0.875	22.2
5-0025	5	0.250	6.4	1.000	25.4
5-0050	5	0.500	12.7	1.250	31.8
5-0075	5	0.750	19.0	1.500	38.1
5-0150	5	1.500	38.1	2.250	57.2
5-0300	5	3.000	76.2	3.750	95.2
5-0600	5	6.000	152.4	6.750	171.4
8-0300	8	3.000	76.2	3.750	95.2
8-0600	8	6.000	152.4	6.750	171.4

amplitude and area-amplitude characteristics is necessary for each application. This use may be inappropriate for other materials and curved surfaces without special compensation. Also see (3) for cautions regarding use of standard blocks for test standardization.

6. Description of Various Recommended Sets

6.1 In ultrasonic testing of aluminum alloy products, a standard reference usually is necessary to establish a specified test sensitivity. A standard ultrasonic reference also is required frequently to determine the effect of variations in metal distance upon the ultrasonic response from detected discontinuities. Test sensitivity standardizations and corrections for metal distance are most reliable when made under the same conditions employed for the actual tests. For these purposes, aluminum alloy reference blocks containing various combinations of hole size and metal distance are necessary.

6.2 The following combinations or sets of blocks are recommended:

6.2.1 *Basic Set*—The basic set consisting of ten reference blocks is listed in Table 1. Area-amplitude relations are obtained by intercomparison of blocks containing the 3-in. (76.2-mm) metal distance and $\frac{3}{64}$ -in., $\frac{5}{64}$ -in., and $\frac{8}{64}$ -in. (see Note 3) diameter holes, respectively. Distance-amplitude relations are obtained by intercomparison of the blocks of various lengths which contain $\frac{5}{64}$ -in. diameter holes.

NOTE 3—Direct conversion from inches to millimetres (1 in. = 25.4 mm) gives hole size dimensions for which there are no standard metric drills; however, Table 2 gives the nearest standard metric drill size.

6.2.2 *Area-Amplitude Set*—The area-amplitude set consisting of eight ultrasonic standard reference blocks is listed in Table 3. Area-amplitude relationships are obtained by intercomparison of any three or more blocks with different flat bottom-hole sizes at the same metal distance from front surface to hole bottom.

6.2.3 *Distance-Amplitude Set*—A distance-amplitude set may include any convenient number of the reference blocks shown in Table 4 and does not necessarily include all blocks listed. A recommended distance-amplitude set contains at least 12 blocks, and each set contains only one of the three hole sizes shown in Table 4. Blocks comprising the 19 block distance-amplitude sets, which are customarily supplied commercially,

⁴ Measurement services to determine the ultrasonic response of reference blocks intended to meet the requirements of this practice are available from several commercial testing laboratories.

TABLE 2 Diameter of Flat-Bottom Holes in Inch-Pound Units and the Nearest Metric Drill Hole Diameter

NOTE 1—Ratio of the area of the nearest metric drill size to the area of the inch-pound drill size is 1.016 throughout.

Hole Diameter in Inch-Pound Units, in.	Nearest Metric Drill Size, mm
1/64	0.40
2/64	0.80
3/64	1.20
4/64	1.60
5/64	2.00
6/64	2.40
7/64	2.80
8/64	3.20

TABLE 3 Dimensions and Identification of Reference Blocks in the Area-Amplitude Set (see Fig. 1)

Block Identi- fication Number	Hole Diameter (A)	Metal Distance (B)		Overall Length (C)	
	¹ / ₆₄ ths in.	in.	mm	in.	mm
1-0300	1	3.000	76.2	3.750	95.3
2-0300	2	3.000	76.2	3.750	95.3
3-0300	3	3.000	76.2	3.750	95.3
4-0300	4	3.000	76.2	3.750	95.3
5-0300	5	3.000	76.2	3.750	95.3
6-0300	6	3.000	76.2	3.750	95.3
7-0300	7	3.000	76.2	3.750	95.3
8-0300	8	3.000	76.2	3.750	95.3

are indicated in Table 4. Increments of metal distance in each of the three groups of blocks in the recommended set should be identical. Distance-amplitude relationships are obtained by intercomparison of all blocks containing the same size hole.

6.3 If the blocks are to be used for immersion testing, they should be suitably anodized or otherwise protected to enhance resistance to corrosion. Blocks with coated surfaces may be used with search units requiring external ground provided suitable arrangements are made for adequate electrical contact. Uncoated blocks shall be designated as Type 1; coated blocks shall be designated as Type 2. The ultrasonic characteristics of both types shall be checked by the immersion method as prescribed in Section 11. However, care must be exercised to dry the Type 1 blocks subsequent to immersion in water. The protective coating used on the Type 2 blocks shall not change their ultrasonic characteristics.

6.4 A number of important variables that affect the response from reference blocks can be controlled during fabrication by accurate machining practices. The roughness of the entry surface; the alignment of entry surface, hole bottom, and back surface; and the surface condition of the hole bottom are the more important physical variables that must be controlled during the fabrication of reference blocks. The quality of material used for blocks also is a factor.

7. Material

7.1 The recommended material for reference blocks is 7075-T6 aluminum alloy rolled or extruded rod (see 13.2).

NOTE 4—To normalize ultrasonic transmission characteristics, the bar stock may be re-heat treated *prior* to manufacturing the blocks. If this

TABLE 4 Dimensions and Identification of Reference Blocks in Distance-Amplitude Sets (see Fig. 1 and refer to 6.2.3)

Block Identification Number, 3-, 5-, and 8- ^A	Metal Distance (B)		Overall Length (C)	
	in.	mm	in.	mm
–0006 ^B	0.0625	1.6	0.812	20.6
–0012 ^B	0.125	3.2	0.875	22.2
–0025 ^B	0.250	6.4	1.000	25.4
–0038 ^B	0.375	9.5	1.125	28.6
–0050 ^B	0.500	12.7	1.250	31.8
–0062 ^B	0.625	15.9	1.375	34.9
–0075 ^B	0.750	19.1	1.500	38.1
–0088 ^B	0.875	22.2	1.625	41.3
–0100 ^B	1.000	25.4	1.750	44.5
–0125 ^B	1.250	31.8	2.000	50.8
–0150	1.500	38.1	2.250	57.2
–0175 ^B	1.750	44.5	2.500	63.5
–0200	2.000	50.8	2.750	69.9
–0225 ^B	2.250	57.2	3.000	76.2
–0250	2.500	63.5	3.250	82.6
–0275 ^B	2.750	69.9	3.500	88.9
–0300	3.000	76.2	3.750	95.3
–0325 ^B	3.250	82.6	4.000	101.6
–0350	3.500	88.9	4.250	108.0
–0375 ^B	3.750	95.3	4.500	114.3
–0400	4.000	101.6	4.750	120.7
–0425 ^B	4.250	108.0	5.000	127.0
–0450	4.500	114.3	5.250	133.4
–0475 ^B	4.750	120.7	5.500	139.7
–0500	5.000	127.0	5.750	146.1
–0525 ^B	5.250	133.4	6.000	152.4
–0550	5.500	139.7	6.250	158.8
–0575 ^B	5.750	146.1	6.500	165.1
–0600	6.000	152.4	6.750	171.5

^AHole diameters (A) 3/64, 5/64, and 8/64 in.

^BBlocks customarily included in commercial 19 block distance-amplitude sets.

option is elected, a recommended practice is soaking at 870 ± 10°F (465 ± 5°C) for a period of 1 h ± 5 min, quenching immediately by immersing vertically into water at room temperature, aging in air at room temperature for 4 days ± 1 h, followed by air aging at 250 ± 10°F (120 ± 5°C) for 24 ± 1 h. To minimize distortion during vertical quenching, it is recommended that stock be re-heat treated in lengths of approximately 20 in. (508 mm).

7.2 The stock shall not be less than 2.00 in. (50.8 mm) nor more than 2.25 in. (57.2 mm) in diameter and up to 6.75 in. (171 mm) in length for the blocks covered by this practice.

8. Quality of Material

8.1 The quality of material to be used for reference blocks should be checked by the procedure outlined in 8.2 to 8.9 inclusive. Only material passing the requirements given in 8.9 should be used for blocks.

8.2 *Evaluation Procedure*—The general evaluation procedure consists of directing a beam of pulsed longitudinal waves into the stock in a diametrical direction and noting the ultrasonic noise level. An ultrasonic test by the immersion method using clean water that is free of air bubbles as a couplant is employed for this evaluation.

8.3 *Test Instrument*—Any of several commercially available pulse-echo type ultrasonic testing instruments that provide a 10-MHz test frequency may be used for evaluation of stock quality. The instrument should be capable of providing the required sensitivity level with negligible internal electrical noise and should provide linear amplification of received pulses in an amplitude range of at least 50 % of maximum amplitude of indication on its display screen.

8.4 Test Frequency—The test frequency to be used for evaluation of the quality of the reference block material shall be 10 MHz.

8.5 Search Unit—An immersion type search unit containing an 0.38-in. (9.5-mm) diameter piezoelectric transducer attached to an appropriate search tube shall be used.

8.6 Immersion Equipment—The required pieces of auxiliary equipment are as follows:

8.6.1 A tank of sufficient capacity to facilitate testing of stock.

8.6.2 A search unit holding and manipulating device.

8.6.3 A suitable traversing bridge to provide angulation and lateral positioning of the search unit.

8.7 Adjustment of Sensitivity—Determine test sensitivity by directing the ultrasonic beam to an 0.1875-in. (4.8-mm) diameter steel ball, of ball bearing quality, attached to a suitable holding device which is immersed in the water. The water distance to the ball (crystal surface to ball surface) should be equal to the measured Y_0^+ of the transducer. Manipulate the search tube to obtain a maximum indication from the ball. Then set the amplitude of this indication by suitable adjustment of the sensitivity (or gain) control of the instrument at 50 % of the upper vertical linearity limit of the display.

8.8 Details of Evaluation Procedure—Position the search unit to obtain a maximum number of back reflections through the diameter of the stock using a water distance of equal to the Y_0^+ of the transducer minus the radius of the material. Then scan the test piece longitudinally and observe the maximum height of the ultrasonic noise level. Make another similar longitudinal scan subsequent to rotating the test piece 90°. Check alignment of the search unit periodically during the scans. Proper alignment of the ultrasonic beam with respect to the test piece exists only when a maximum number of back reflections is maintained.

8.9 Basis of Acceptance—The material is acceptable if the maximum magnitude of indications in the ultrasonic noise level does not exceed 20 % of the maximum magnitude of indication obtained from the 0.1875-in. (4.8-mm) diameter steel reference ball. At least five back reflections should be observed at all times during the scanning procedure. Acceptable block material shall not contain discontinuities in excess of the ultrasonic noise level.

9. Procedure for Fabricating Blocks

9.1 Machine reference blocks to a uniform finish within the dimensional tolerances given in 9.2 to 9.10, inclusive, and as specified in Fig. 1. Dimensions of each block are given in Table 1, Table 3, and Table 4.

9.2 Final Diameter of Block—Finish the block to a true diameter of 2 ± 0.020 in. (50.8 ± 0.51 mm) and a surface finish of 63 μ in. (1.6 μ m) rms, or smoother.

NOTE 5—The close tolerance on the diameter is to assure a good fit in the holders that are sometimes used for retaining blocks.

9.3 End Facing—The machined ends shall be flat within 0.0002 in. (0.005 mm) and perpendicular to the longitudinal axis. The two ends shall be parallel within 0.001 in. (0.03 mm).

The surface finish of the entry surface shall be 30 μ in. (0.76 μ m) rms, or smoother, and the back surface 63 μ in. (1.6 μ m) rms, or smoother.

9.4 Hole Alignment—The hole must be perpendicular to the end of the block within a tolerance of 30 min. The hole should be located within 0.010 in. (0.25 mm) of the longitudinal axis of the block.

9.5 Hole Bottom—Make the hole bottom flat by final drilling with a flat-end drill or cutter. The end of the drill or cutter used for this purpose should be flat within 0.001 in. (0.03 mm) per 0.125 in. (3.2 mm) of diameter and should be perpendicular to its longitudinal axis. The final depth of the finished flat-bottom hole is 0.75 in. (19.0 mm). Make the finished hole bottom as smooth as possible.

9.6 Counterbore for Plug—Machine a flat counterbore, 0.250 in. (6.35 mm) in diameter by 0.063 in. (1.62 mm) deep, into the end of the block at its center as shown in Fig. 1.

9.7 Cleaning and Drying Hole—Upon completion of the counterboring and drilling operations, clean the hole bottom with a suitable cleaning fluid and dry with a fine stream of dried, filtered, compressed air blown through a capillary tube inserted in the hole.

9.8 Deburring—Remove all burrs resulting from the machining procedure. Round the outside edges of entry and back surfaces to a radius of not more than 0.032 in. (0.81 mm).

9.9 Block Identification—Identify each reference block by a stenciled block identification number, designating hole size, and metal distance, as given in Table 1, Table 3, and Table 4. In the case of additional and equivalent blocks, as defined in 13.1, which are fabricated to a precise metric system dimension or to mixed English/metric dimensions, the metric dimension shall be indicated by the marking “mm” immediately following the dimension number. For example, a block with a $\frac{5}{64}$ -in. diameter flat-bottom-hole target and a 3 mm metal path would be identified as “5-3 mm” and a block with a 1 mm diameter flat-bottom-hole target and a 1 in. metal path would be identified as “1 mm-0100”. The size and location of the stenciled numbers are indicated in Fig. 1. Take special care to protect the block, particularly the entry surface, from handling marks and scratches during the stenciling operation. Stamp or stencil on the block additional information designating the manufacturer and compliance with this practice (see 11.9). However, this information should be located at a point at least 90° about the periphery from the aforementioned block identification number. Letter size and spacing of this additional information should not be greater than letter size and spacing used for the identification number.

9.9.1 Ink identification may be written on the block sound entry surface provided that it has been established that the markings do not affect the block’s measured echo-amplitude response. Etching, scratching, or physical defacing of the block’s sound entry surface is not permitted.

9.10 Plugging Procedure—Check the completed unplugged reference block for ultrasonic response prior to plugging. Plug a reference block that exhibits satisfactory ultrasonic response by seating an aluminum plug of the same alloy (7075-T6) that has an interference fit of 0.0005 in. (0.013 mm) in the counterbore. Coat both the counterbore and the faying surface

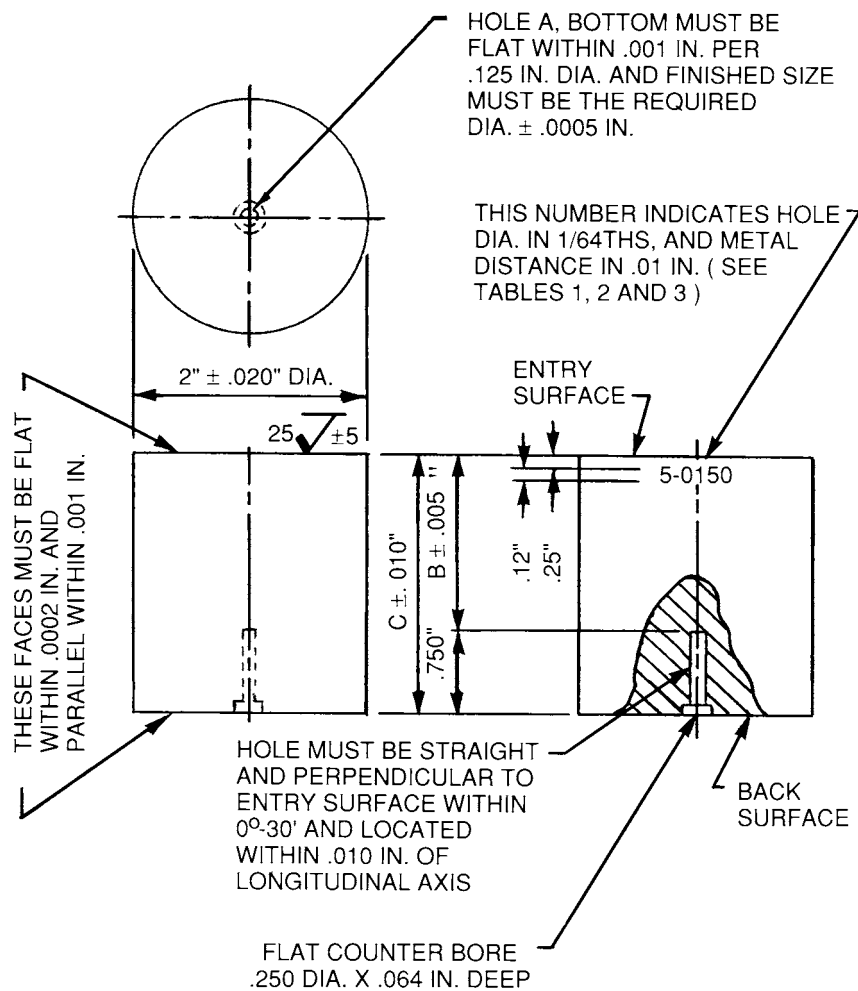


FIG. 1 Ultrasonic Standard Reference Block

of the plug with a permanent water-impervious rubber-base adhesive before the plug is driven into place. The exposed surface of the seated plug can be slightly below, but should not extend above, the surface.

10. Procedure for Checking Physical Characteristics of Blocks

10.1 *Entry Surface*—Check each finished reference block to ensure flatness and parallelism of entry surface and back surface. A dial gage reading to 0.0001 in. (0.003 mm) and a surface plate may be used for this check. A finished reference block exhibiting misalignment greater than 0.001 in. (0.03 mm) or lack of flatness greater than 0.0002 in. (0.005 mm) over the entire entry surface area is not acceptable.

10.2 *Entry Surface Roughness*—Roughness of the entry surface may be checked using any one of several commercially available roughness measuring instruments. The recommended procedure involves moving the roughness detector (scanning device) of the instrument diametrically across the entry sur-

face. Note deviation in surface roughness during the scan. Finished blocks shall have a surface roughness no greater than 30 μ in. (0.76 μ m).

11. Procedure for Checking Ultrasonic Characteristics of Blocks

11.1 *Reasons for Ultrasonic Check*—A fabricated block exhibiting satisfactory external physical characteristics must be subjected to additional ultrasonic tests by the immersion method in order to check the characteristics of the hole and hole bottom. The ultrasonic tests consist of checking the response from the block as well as checking for possible angular error. The block response is a function of smoothness and flatness of the hole bottom. Angular error will result from misalignment of the hole bottom with respect to the entry surface. Because poor response from a fabricated block may be alleviated by additional cleaning of the hole bottom, make the initial ultrasonic check prior to sealing the hole with a permanent aluminum plug.

11.2 *Test Frequency*—Use a test frequency of 5 MHz to check reference blocks.

11.3 *Apparatus:*

11.3.1 *Test Instrument*—Any of several commercially available pulse-echo type ultrasonic testing instruments that employ a *tuned pulse* to provide a test frequency of 5 MHz and that facilitate tests by the immersion method may be used for checking reference blocks. The instrument used should provide stable, linear amplification of received pulses at the required sensitivity levels and should be free of interface signal interference. An appropriate line voltage regulating transformer shall be used to ensure maximum regulation, if not provided internal to the instrument. The instrument calibration shall be checked in accordance with the procedure outlined in 11.4.

11.3.2 *Tank*—Any container is satisfactory that will facilitate the accurate positioning of the reference blocks being checked, the fundamental standard reference balls, and the search unit.

11.3.3 *Manipulator and Bridge*—If a manipulator is used, it should adequately support a search tube and should provide fine adjustment of angle within 1° in two vertical planes that are normal to each other. The bridge should be of sufficient strength to support the manipulator rigidly and should allow smooth accurate positioning of the search unit. Special fixtures may be used provided they meet the requirements prescribed for a manipulator and bridge.

11.3.4 *Couplant*—Clean water, free of air bubbles, should be used as a couplant. Inhibitors or wetting agents, or both, may be used if it is established that their use does not alter the ultrasonic characteristics of the couplant. However, it is important that the same water, at the same temperature, be used for comparing the response from different reference blocks.

11.3.5 *Search Unit*—An immersion search unit having the performance characteristics described in 11.5 shall be used. It shall comprise a flat, round, piezoelectric transducer element of any suitable material and beam characteristics resonant at 5.0 MHz, with an effective diameter as required to produce a last near field maximum (Y_0^+) in the range of 3.2 to 3.6.

NOTE 6—During the development of this practice, search units with quartz elements having the following dimensions were used:

(1) element diameter—0.5 in. (12.7 mm)

(2) back electrode diameter—0.375 in. (9.53 mm)

(3) front electrode—entire face and edge to provide 360° ground connection

These and later similar units conforming to this practice, are often referred to as having a “3/8-in. effective diameter.”

11.4 *Qualification of Test System:*

11.4.1 *Reasons for Qualification*—Because differences usually exist in the amplification characteristics of receivers or echo-amplifiers in various test instruments, changes in the amplitude of ultrasonic indications might not be displayed linearly over the entire readable range on the screen of a test instrument. In order to establish correctly the required characteristics of the test system used to check reference blocks, it is necessary to determine the actual linear range of the test system.

11.4.2 *Apparatus*—The same apparatus, including the test instrument, tank and manipulator, and search unit prescribed for checking reference blocks (see 11.3) shall be used to check the linearity of the test system if Method A of Practice E317 is used to check linearity.

11.4.3 *Procedure for Checking Linearity*—Determine the vertical linearity characteristics of the test system in accordance with either Method A or Method B of Practice E317. For checking the response of reference blocks, use only that portion of the vertical instrument deflection that lies within $\pm 5\%$ of a constant response ratio. This will define the upper and lower linearity limit.

11.5 *Qualification of Search Unit:*

11.5.1 *Reasons for Qualification*—In order to ensure maximum accuracy during the check of block response, check the characteristics of the search unit and use only search units exhibiting acceptable characteristics for this work. The characteristics of the search unit include the following:

11.5.1.1 Frequency,

11.5.1.2 A distance-amplitude curve from a 0.500-in. (12.7-mm) diameter steel ball in water, and

11.5.1.3 Beam profiles obtained from a 0.500-in. (12.7-mm) diameter ball in water.

11.5.1.4 Any piezoelectric material that enables the search unit to meet the requirements of this practice may be used.

11.5.2 *Apparatus*—The apparatus used for checking the ultrasonic characteristics of the search unit is the same as that prescribed in 11.3 for checking reference blocks. The manipulator should allow a range in water path from 0 to at least 6 in. (152.4 mm). The steel balls required shall be of ball-bearing quality, free of corrosion and surface marks.

11.5.3 Verify the center frequency of the search unit and system to be 5.0 ± 0.5 MHz.

11.5.4 *Procedure for Obtaining Distance-Amplitude Characteristics*—Obtain an initial response from a 0.500-in. (12.7-mm) diameter steel ball that is located at a water distance equal to the measured Y_0^+ of the search unit. Position the search unit for a maximum indication from the ball under these conditions. Take care to obtain a true maximum indication because the position of the search unit is critical. Subsequent to obtaining the maximum response, adjust the instrument gain control to bring this response to 100 % of the upper linearity limit of the instrument. Then vary the water distance in increments no greater than 0.25 in. (6.4 mm) through a range from 0.25 in. (6.4 mm) to the Y_0^+ point, and from this point in increments no greater than 0.5 in. (12.8 mm) to 6 in. (152.4 mm). Because only the axial distance-amplitude response is required, take care to maintain the location of the ball on the central axis of the beam for each increment of water distance. Plot the incremental response from the ball as a function of water distance. A typical response curve for an acceptable search unit is shown in Fig. 2. Only a search unit with a measured Y_0^+ point at 3.2 to 3.6 in. (81 to 91 mm) and a distance-amplitude curve similar to that shown in Fig. 2 will display sets of amplitude response curves equivalent to those required by 11.8.1 and 11.8.2.

11.5.5 *Procedure for Obtaining Beam Patterns:*

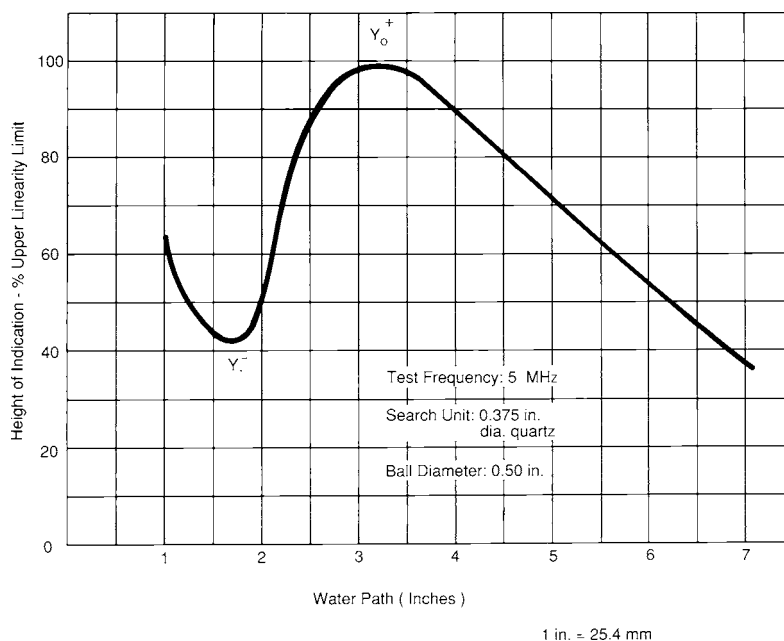


FIG. 2 Typical Axial Distance-Amplitude Characteristics of an Acceptable Search Unit

11.5.5.1 Obtain the beam characteristics from a 0.500-in. (12.70-mm) diameter steel ball immersed in water at a distance equal to the last maximum amplitude point as determined in 11.5.4. This is the point labeled Y_0^+ in Fig. 2. This plot is obtained by observing the height of indication from the ball while the ball passes under the search unit along its diameter. One distinct lobe or maximum should be observed. An acceptable search unit will give a beam profile with no significant side lobes, as shown in Fig. 3. Check the beam profile symmetry by making four scans, each scan displaced 45° in a plane parallel to the search unit face. This beam profile will determine the beam diameter of the search unit. The dimensions of the beam will be determined at the 50 % (6 dB down) amplitude point. The beam diameter of an acceptable search unit must have a minimum ratio of 0.75:1 when the minimum beam size obtained from the four scans is divided by the maximum beam size obtained from the four scans.

11.5.5.2 Make a second series of beam profiles at a water distance equal to the measured Y_1^- point (approximately one half of the water path used for the beam dimensional profile). This plot is obtained by observing the height of indication from the ball while the ball passes under the search unit along its diameter. Two distinct lobes or maximums should be observed, as shown in Fig. 4. Check this series of profiles by making four scans at the same sensitivity, each scan displaced 45° in a plane parallel to the search unit face. An acceptable search unit will have an amplitude variation no greater than 15 % between maximum points for all four scans. These profiles determine the beam pressure symmetry of the search unit.

11.6 Preparation of Blocks for Ultrasonic Check—Check the hole bottom and entry surface of the block for cleanliness. An additional cleaning of the hole bottom with a suitable cleaning fluid followed by drying with dried, compressed air may be necessary. Use a temporary seal to protect the hole, which is not permanently plugged during the initial ultrasonic

check. Any good water-impervious adhesive tape affixed to the back surface over the hole can be used as a temporary seal.

11.7 Procedure for Checking Angular Error:

11.7.1 Direct the search unit toward the reference block that is immersed in the water at a 3.5-in. (88.9-mm) distance from the face of the search unit. Accurately adjust this distance (within $\pm 1/32$ in. or 1 mm) by using a gage between the block and the crystal. Adjust the angle of the search unit with respect to the block to obtain either a maximum number of back reflections from the block or a maximum indication from its entry surface.

11.7.2 After a normal ultrasonic beam is obtained, position the search unit laterally to obtain a maximum response (in the linear range) from the hole bottom. When maximum response has been obtained in this manner, angulate the search unit through a small angle in two mutually perpendicular planes and note any increase in the height of indication from the hole bottom. A reference block is acceptable if any increase in response from the hole bottom obtained by angulating the search unit is less than 10 % of the initial magnitude of indication obtained with a perpendicular beam.

11.8 Procedure for Checking Ultrasonic Response—Direct the search unit toward the reference block that is immersed in the water at a distance equal to the measured Y_0^+ distance of the search unit from the crystal face to the block entry surface. An exception to this procedure is to continue the use of a previous practice in cases where experience with a given search unit and a given set or sets of blocks has yielded satisfactory results by using a water path of 3.5 ± 0.1 in. (88.9 $\pm$ 2.5 mm) even though different from the measured Y_0^+ of a search unit meeting the other requirements of 11.5. Accurately adjust this water distance by using a gage between the block and the search unit. Adjust the angle of the search unit with respect to the block to obtain either a maximized number of back reflections from the block or a maximized indication from

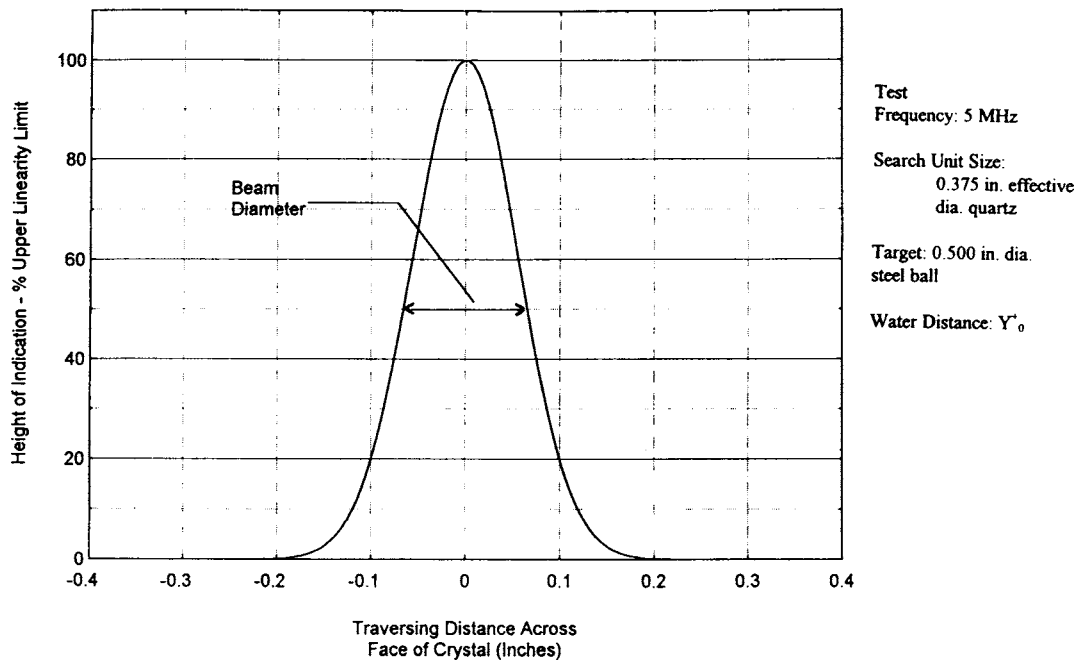


FIG. 3 Beam Characteristics of an Acceptable Search Unit at Y_0^+ Point

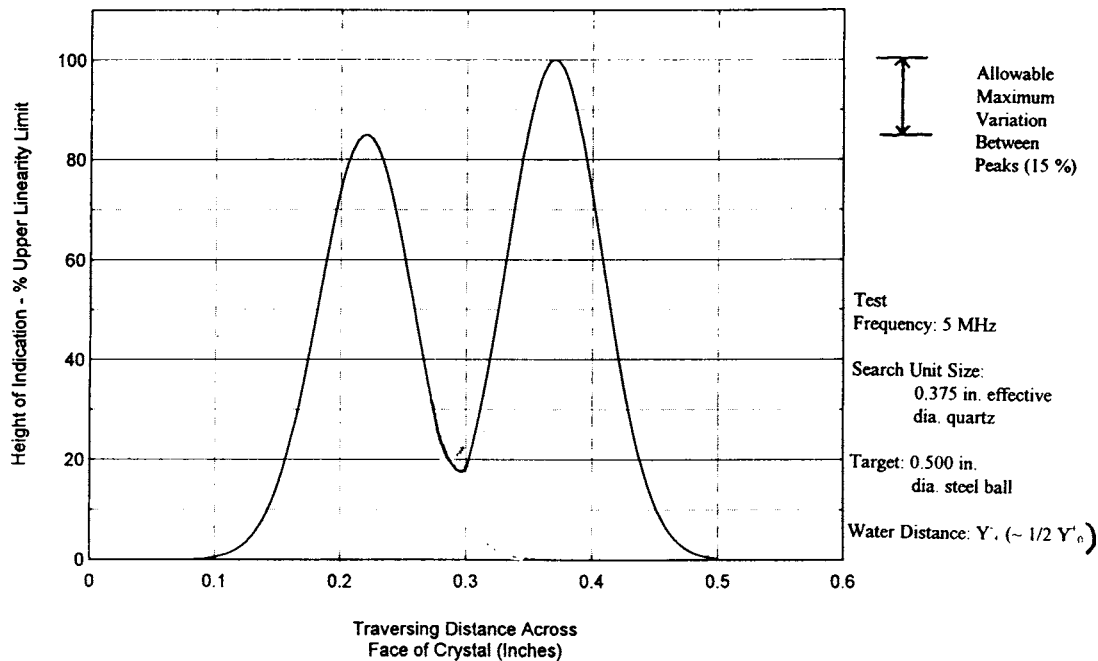


FIG. 4 Beam Characteristics of an Acceptable Search Unit at Y_1^- Point

its entry surface. After a normal ultrasonic beam is obtained, position the search unit laterally and re-angle slightly as required to obtain a maximized amplitude of indication from the hole bottom. Test each block in an area-amplitude set or distance-amplitude set in this manner, and plot curves similar to Fig. 5 and Fig. 6 for each set. Alternative methods for obtaining the required amplitude response data (such as the use of calibrated gain controls) may be used, provided the reading accuracies specified in 11.4.3 and 11.8.2.2 are maintained. The

detailed procedures described later require the calibration of test system sensitivity. This may be done either with the ball-to-block method of 11.8.2 or the block-to-block method of Annex A1 or the interface-to-block method of Annex A2. The method used and the data obtained, as well as the prescribed curves, should be included in the test report. An exception to this procedure is to continue the use of a previous practice in cases where experience with a given search unit and a given set or sets of blocks has yielded satisfactory results by using a

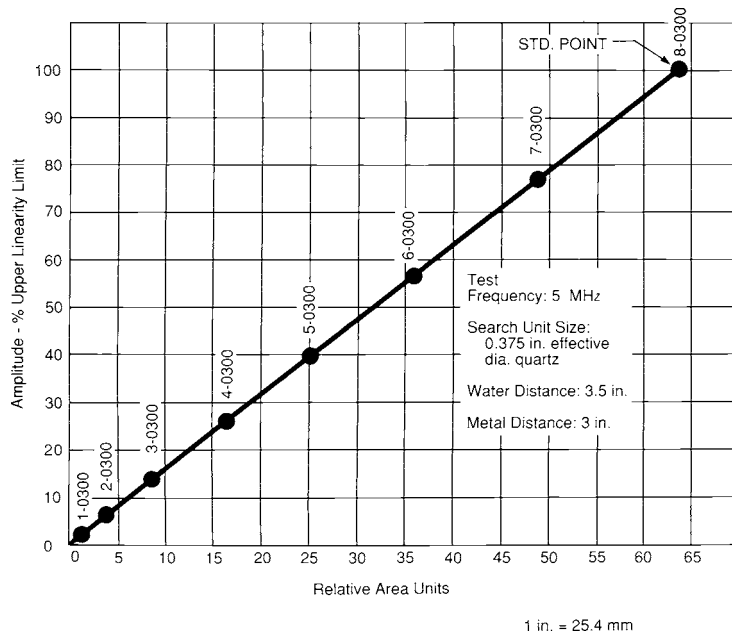


FIG. 5 Area-Amplitude Response Curve Showing Interrelationship Between Ultrasonic Standard Reference Blocks Containing Holes of Various Sizes at Constant Metal Distances

DISTANCE - AMPLITUDE PLOT

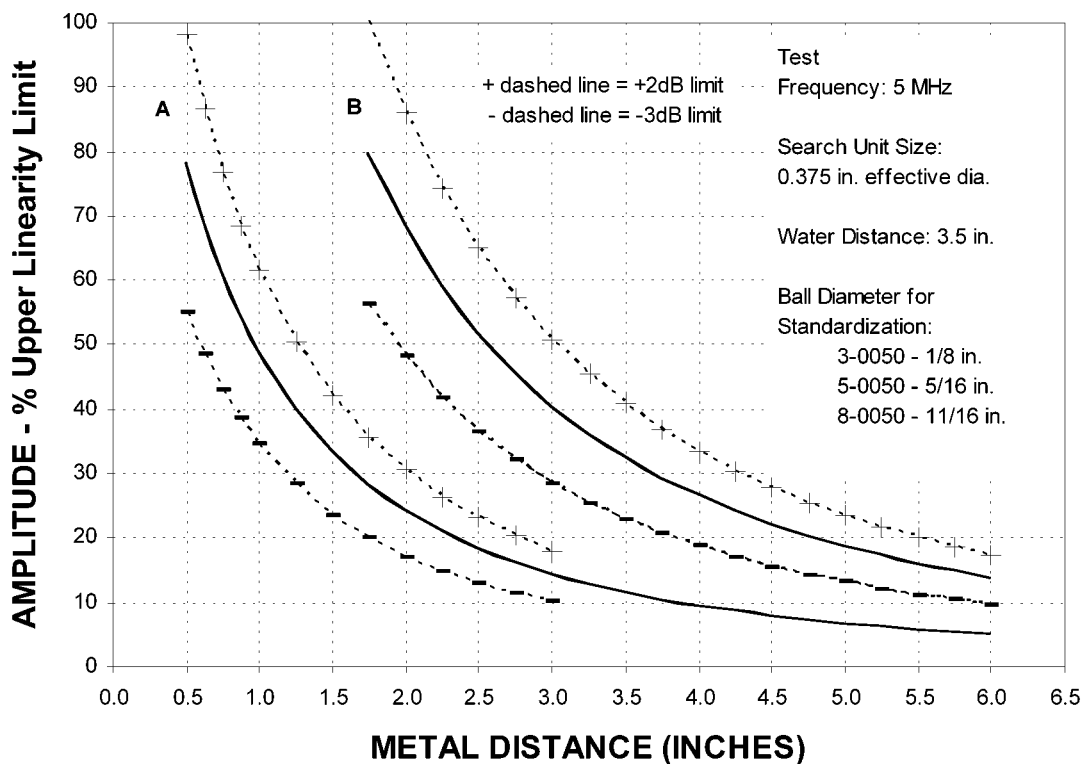


FIG. 6 Distance-Amplitude Response Curves (A and B) Showing the Interrelationship Between Ultrasonic Standard Reference Blocks of Various Lengths and Containing Flat-Bottom Holes

water path of 3.5 ± 0.1 in. (88.9 ± 2.5 mm) even though this water path length is different from the measured Y_0^+ of a search unit meeting the other requirements of 11.5.

11.8.1 *Area-Amplitude Set*—Establish test sensitivity for the area-amplitude curve shown in Fig. 5 by adjusting the instrument gain control so that the maximized indication from the

TABLE 5 Comparison Data for Checking Ultrasonic Response of Standard Reference Blocks (see Fig. 6)

NOTE—All indicated values, including the Curve A and Curve B values, have been rounded to the nearest 0.5 dB from the corrected NIST formula. This accounts for the small differences in the +2 dB and -3 dB listed values from those that are obtained if they are calculated from the listed A and B values, which themselves have been rounded to the nearest 0.5 dB. The listed min and max values are calculated from the formula values and are correct, but should be used with the stated $\pm 2\%$ FS reading error allowances as stated in Note 7.

Block Identification Number	Block Response ^A	Allowable Variation ^A		Block Response ^A	Allowable Variation ^A	
	Curve A	min (-3dB)	max (+2dB)	Curve B (A + 9dB)	min (-3dB)	max (+2dB)
0050	78.0	55.5	98.5			
0063	68.5	48.5	86.5			
0075	61.0	43.0	77.0			
0088	54.5	38.5	68.5			
0100	49.0	34.5	61.5			
0125	40.0	28.5	50.5			
0150	33.5	23.5	42.0			
0175	28.5	20.0	35.5	79.5	56.5	100.5
0200	24.0	17.0	30.5	68.5	48.5	86.0
0225	21.0	15.0	26.5	59.0	42.0	74.5
0250	18.5	13.0	23.0	51.5	36.5	65.0
0275	16.0	11.5	20.5	45.5	32.0	57.5
0300	14.5	10.0	18.0	40.5	28.5	51.0
0325				36.0	25.5	45.5
0350				32.5	23.0	41.0
0375				29.0	20.5	37.0
0400				26.5	19.0	33.5
0425				24.0	17.0	30.5
0450				22.0	15.5	28.0
0475				20.5	14.5	25.5
0500				18.5	13.0	23.5
0525				17.0	12.0	21.5
0550				16.0	11.5	20.0
0575				15.0	10.5	18.5
0600				14.0	10.0	17.5

^APercent upper linearity limit.

$\frac{5}{64}$ -in. diameter hole (Block 8-0300) is equal to or less than the upper linearity limit. Then obtain the maximized indication from each block in the set (see Table 4) at this sensitivity level, and plot results as shown in Fig. 5. A set of blocks meeting the requirements of this practice will give an approximately linear, monotonic relationship (that is, no negative slope direction between points) between indication height and relative flat-bottom hole area as shown in Fig. 5 within +2, -3 dB $\pm 2\%$ of upper linearity limit.

NOTE 7—To maintain a consistent relationship between blocks in area-amplitude, distance-amplitude, and basic sets, all blocks having $\frac{3}{64}$ in., $\frac{5}{64}$ in., and $\frac{7}{64}$ in. diameter holes, must conform to the response requirements of Table 5 when evaluated by the procedures of 11.8.2. Reference to “requirements of Table 5” include the $\pm 2\%$ of upper linearity limit. This applies to Distance-amplitude sets, Area-amplitude sets, and Basic sets.

11.8.2 Distance-Amplitude Set—Test sensitivity for the distance-amplitude curves shown in Fig. 6 is established by adjusting the instrument gain control so that the response from a steel reference ball is equal to 80 % of the upper linearity limit of the test system. Alternatively, test sensitivity may be established by the method described in Annex A2

NOTE 8—Because entry surface resolution obtained at the specified test frequency of 5 MHz may be limited to 0.500 in. (12.70 mm) for aluminum

alloys, blocks with metal distances of less than 0.500 in. may not be able to be checked in accordance with this recommended practice depending upon the type of search unit and instrument employed.

11.8.2.1 For reference blocks having a flat-bottom hole of $\frac{3}{64}$ in. in diameter, establish the sensitivity by using a $\frac{1}{8}$ -in. (3.2-mm) diameter ball using a water path of 3.5 ± 0.1 in. (88.9 ± 2.5 mm). Carefully manipulate the search unit over the ball to obtain the maximum amplitude of response. The gain during this adjustment should be such that the response is always less than the upper linearity limit. When the maximum response has been obtained, increase the gain to give an amplitude equal to 80 % of the upper linearity limit. Maintaining this sensitivity, obtain the maximum response from each block in the set, and plot the amplitude versus metal distance as shown in Curve A of Fig. 6. Table 5 gives the percent block response for each block from 0050 to 0300.

11.8.2.2 Since the amplitude of response for metal distances over 2.5 in. (63.5 mm) becomes small, better accuracy can be obtained by increasing the instrument sensitivity for the larger metal distances (see Curve B of Fig. 6). Manipulate the search unit over the 0175 block to obtain a response as close as possible to 28.5 % of the upper linearity limit (see Note 9). Using the sensitivity control, raise this 28.5 % to the original 80 % upper linearity limit. An accurately calibrated gain control increase of 9 dB accomplishes this increase to satisfactory accuracy. Maintain this sensitivity level and obtain the maximized response from each block in the set (see Table 4) and plot amplitude versus metal distance as shown in Curve B of Fig. 6. Table 5 gives the percent block response for each block from 0175 to 0600.

NOTE 9—If the response of this block is less than 28.5 %, use of any other block that can be manipulated to give a response of 28.5 % is satisfactory.

11.8.2.3 For reference blocks having a flat-bottom hole $\frac{5}{64}$ in. in diameter, establish the test sensitivity by using a $\frac{5}{16}$ -in. (7.9-mm) diameter ball. Then repeat the procedures of 11.8.2.1 and 11.8.2.2 for all blocks in the set.

11.8.2.4 For reference blocks having a flat-bottom hole $\frac{7}{64}$ in. in diameter, establish the test sensitivity by using an $\frac{1}{16}$ -in. (1.75-mm) diameter ball. Then repeat the procedures of 11.8.2.1 and 11.8.2.2 for all blocks in the set.

11.8.2.5 Indications from blocks meeting the requirements of this practice shall not deviate more than +2, -3 dB, plus the $\pm 2\%$ of upper linearity limit reading error tolerance (See Note 7) from the indicated response described by the curves in Fig. 6 for the percent block response given in Table 5. In addition to the test information shown in Fig. 6, each data sheet should include the type of instrument employed.

11.8.3 Basic Set—The amplitude of response for each block in the basic set (see Table 1) shall comply with the previously described requirements in 11.8.1 and 11.8.2 as follows: Blocks 3-0300, 5-0300, and 8-0300 shall show the response given in Fig. 5 and Blocks 5-0050 through 5-0600 shall show the response given in Fig. 6.

11.9 Reference blocks exhibiting dimensional characteristics of Sections 9 and 10 and response characteristics of 8.9, 11.7, and 11.8 may be permanently sealed with the aluminum plug as previously described. Only such blocks may be

permanently stenciled to reference Practice E127. A final check of ultrasonic characteristics is recommended after the blocks are plugged.

12. Report

12.1 Report the following information:

12.2 *Equipment Used*:

12.2.1 Instrument: manufacturer, type, modules (where applicable) and serial numbers.

12.2.2 Search unit: manufacturer, type, part number, and serial number.

12.2.2.1 Certify that both the search unit and test system meet the requirements of 11.4 and 11.5.

12.3 *Area/Amplitude Block Sets*:

12.3.1 Numerical response values obtained by procedure 11.8.1.

12.3.2 Provide data plot in accordance with Fig. 5.

12.3.3 For 3-0300, 5-0300 and 8-0300 blocks, report numerical values obtained by the procedures in 11.8.2 or Annex A1.

12.4 *Distance/Amplitude Block Sets*:

12.4.1 Numerical values obtained by procedure 11.8.2 or Annex A1.

12.4.2 Provide data plot in accordance with Fig. 6.

12.5 *Basic Sets*:

12.5.1 For 3-0300, 5-0300 and 8-0300, follow 12.3.

12.5.2 For all other blocks follow 12.4 for applicable metal distances.

12.6 *Blocks Not in Sets*—Unless otherwise specified by the requesting party, for blocks with $\frac{3}{64}$, $\frac{5}{64}$ or $\frac{8}{64}$ in. diameter FB holes, report numerical values obtained by the procedures in 11.8.2 or Annex A1.

NOTE 10—Response limits are given by Table 5 for blocks with metal distances of 0.5 in. (12.7 mm) to 6.0 in. (152 mm) and having $\frac{3}{64}$, $\frac{5}{64}$ or $\frac{8}{64}$ in. diameter FB holes. Blocks having other hole sizes or metal distances may be evaluated by the procedures in 11.8.2 or Annex A1, but reporting format and response limits must be established by the using parties.

13. Additional and Equivalent Blocks

13.1 Additional blocks can be used, where advantageous, to supplement the recommended sets. If additional blocks are fabricated, their ultrasonic response should conform to the area-amplitude and distance-amplitude interrelationships defined by the curves in Fig. 5 and Fig. 6.

13.2 Practice E127-type blocks that were fabricated and checked prior to the issuance of Practice E127-75 should be requalified in accordance with the procedures described in the latest edition of this practice.

13.3 Numerous blocks are now in use that do not meet all the requirements prescribed in this recommended practice (for

instance, other aluminum alloys). They may be considered equivalent to the ASTM Aluminum Alloy Ultrasonic Standard Reference Blocks if they meet the ultrasonic response requirements given in 11.8.

13.4 Blocks that do not meet the ultrasonic response requirements given in 11.8 are not considered equivalent to the ASTM Aluminum Alloy Ultrasonic Standard Reference Blocks. If they meet all other requirements, and if a correction curve or table is furnished with these blocks so that their amplitude of response can be corrected to give a response equivalent to the requirements of this recommended practice, they may be considered ASTM-type reference blocks.

13.5 Excessive wear and use may require the occasional introduction of a newly-fabricated block into an existing set. These replacement blocks must meet all of the requirements of this standard and be acoustically similar to the block(s) being replaced. For the purposes of being acoustically similar, these blocks must meet the Table 5 measurement criteria and have an appropriate relative echo-amplitude response with respect to the other blocks in the existing block set.

13.6 An exception to the requirements of 13.2, 13.3, and 13.4 for acceptance of additional blocks exists in the case of blocks that meet all other requirements of this practice except that they produce, at some metal path distances, higher amplitude responses from flat bottom holes than the upper limit figures of Table 5 due to their fabrication from material of lower ultrasonic attenuation. If these blocks were certified as acceptable under an earlier version of this practice, they may be considered acceptable under the criteria of the current version if they are used to test material that can be shown to have similar low attenuation. Recertification of such blocks must show conformance to all requirements of this Standard Practice except the Table 5 upper limits.

14. Technical Precaution

14.1 When Practice E127-type reference blocks are used for transfer or penetration comparisons caution is recommended. Backwall reflection amplitude measurements may be influenced by sidewall reinforcement or edge-to-center differences in metallurgical structure. Practice E127-type blocks were designed primarily for flat-bottomed hole amplitude response comparisons in flat surface material of 2 in. width or greater. Recent work has suggested that a more appropriate use is in determining comparisons and consistency of characteristics of instruments and transducers. (see (Ref. 3)). Caution must be exercised when using these blocks for other purposes.

15. Keywords

15.1 aluminum reference blocks; area-amplitude calibration blocks; distance-amplitude calibration blocks; nondestructive testing; standard reference blocks; ultrasonic reference blocks



ANNEXES

(Mandatory Information)

A1. ALTERNATIVE BLOCK-TO-BLOCK CALIBRATION METHOD

A1.1 Introduction

A1.1.1 This Annex defines a procedure for ultrasonic testing and qualification of aluminum alloy standard reference blocks using as calibration standards, blocks which have been certified by the National Institute of Standards and Technology (NIST) and have been preserved for this sole purpose. The procedure may be used as an alternative to the ball-to-block method of 11.8.2.

A1.2 Application

A1.2.1 The objective is to allow the use of commercially available pulse-echo instrumentation which may not reproduce the ball/block response given in Table 5 to the required tolerances.

NOTE A1.1—The equipment originally used to obtain the response data has not been manufactured for many years, and maintenance of the obsolete instruments has become difficult and expensive.

A1.3 Method

A1.3.1 Blocks which meet all the requirements of this practice except for having been ultrasonically checked for ball-to-block response, are evaluated against similar standard reference blocks which have been calibrated and certified by NIST in accordance with 11.8.2. For the source of this calibration service, see footnote 4.

A1.3.2 Relevant instrumentation parameters are defined and measured.

A1.3.3 Block response acceptance criteria are specified.

A1.4 Apparatus

A1.4.1 The immersion test equipment described in 11.3 and meeting the requirements of 11.4, shall be used.

A1.4.2 To produce the tuned electrical pulse specified in 11.3.1, an appropriate network is necessary if the instrument incorporates a conventional “spike” or “square-wave” pulser. This network must inductively shunt-tune the cable and search unit capacitance to generate the required 5.0 MHz electrical wave-train, and provide the system pulse-echo sensitivity needed for the reference blocks to be evaluated. A suggested network configuration is shown in Appendix X1.

A1.4.3 The combination of pulser, cables, search unit, and control settings used for block evaluation must be checked with standard CRO measurement techniques to ensure that the electrical signal applied to the search unit is a damped sine wave with an effective r-f frequency of 4.8 to 5.2 MHz.

NOTE A1.2—Procedures for making pulser wave-train and receiver bandwidth measurements are described in Guide E1324.

A1.4.4 To approximate the receiver characteristics of the earlier instruments, the peak frequency response shall be within 4.8 to 5.2 MHz, and the receiver bandwidth within 20 to 40 % (@ -3 dB). Both should be checked with the methods cited in Note A1.2, and any required adjustments made in accordance with the instrument manufacturer’s recommendations.

A1.5 Calibration Blocks

A1.5.1 Blocks to be used as calibration standards must be fabricated and evaluated in accordance with, and meet all the requirements of this practice, including Section 11.

A1.5.2 A certified block having the same hole size and metal distance as the specific block to be evaluated must be used.

A1.6 Procedure

A1.6.1 Using the procedure described in 11.7, check the new blocks for angular error to determine that 11.7.2 is satisfied.

A1.6.2 Using the procedure described in 11.8, optimize the search unit alignment with the calibration block and scan laterally to peak on the hole. Adjust the instrument sensitivity to obtain a hole signal equal, in percent of full scale (FS), to that given in the NIST calibration data. This will usually require the use of a fine gain control, and should be set within the readability of the display, that is, 2 % FS or better.

A1.6.3 Without changing sensitivity, repeat the measurement on the block being evaluated, and record the value obtained (in percent FS). For blocks which require response values for both Curve A and Curve B, repeat A1.6.2 and A1.6.3 using the second NIST calibration value.

A1.7 Acceptance Criteria

A1.7.1 The response of acceptable blocks must fall within the tolerances given in Table 5. To meet the report requirements of 12.1, the response values must be plotted in accordance with Fig. 6, and meet the +2 dB and -3 dB limits specified.

A1.7.2 Blocks meeting these response criteria, and all other requirements of this practice other than the ball-to-block evaluation, may be certified as conforming to this practice.

A1.8 Report

A1.8.1 In addition to the information required by 12.1 and 12.2, the report shall show the serial numbers of the calibration blocks used, the corresponding reference response values provided by NIST, and the numerical results on the blocks being tested.

A1.9 Precision and Bias

A1.9.1 An interlaboratory study was made to determine the reproducibility of this method and the relationship of the results to the NIST calibration readings.⁵

A1.9.2 Reproducibility of the average of three or more readings at a single facility using the same instrumentation can be expected to be within 2 % FS.

⁵ Supporting data are available from ASTM Headquarters. Request research report RR:E07-1000.

A1.9.3 The maximum deviation of averaged data from any facility should not deviate from the NIST calibration response by more than 5 % FS.

A1.9.4 Since there is no recognized primary standard against which the response of the ultrasonic reference blocks can be compared, no statement can be made regarding the bias of these measurements.

A2. ALTERNATIVE CALIBRATED GAIN CONTROL METHOD FOR DISTANCE-AMPLITUDE CHECKING

A2.1 Introduction

A2.1.1 This annex defines a procedure for performing distance-amplitude checks without using round balls as the sensitivity reference. This alternate method requires that the vertical linearity and gain control(s) of the instrument be calibrated with an external step attenuator. Linearity checking by this means is described in Method B in Practice E317. Gain control checking is performed by using the same system configuration as shown for vertical linearity checking and by following the procedure described below.

A2.2 Application

A2.2.1 The objective of this procedure is to provide a method for obtaining accurate distance-amplitude checking of reference block sets while using measuring equipment with NIST-traceable accuracy. As is the case with Annex A1 procedures, this method allows the use of newer, readily available ultrasonic pulse-echo instruments that are more stable, linear and accurate than the older instruments originally used for block checking.

A2.3 Equipment Requirements

A2.3.1 The external step attenuator used in this procedure must meet the specification requirements for the attenuator used for the vertical linearity check per Method B of Practice E317. In addition its accuracy must be established at least within one year of each use by means traceable to NIST.

A2.3.2 *Instrument Linearity*—For this procedure instrument linearity must be checked in accordance with Method B of Practice E317, using either the one or two search unit procedures and be within the accuracy specified therein.

A2.3.3 *Gain Control Accuracy*—The procedure described in Guide E1324 in the section labeled “dB Controls” may be used for checking instrument gain control accuracy if, by this means, the accuracy can be determined to be within ± 5 % of the upper vertical linearity limit. An alternate and preferable method is performed by using the same system configuration as was used for the vertical linearity check. If the linearity is within the prescribed ± 5 % limits the steps below are to be followed to check gain control accuracy.

A2.3.3.1 Set the external attenuator to produce 20 dB attenuation.

A2.3.3.2 Set a 5 MHz search unit normal to the surface of a flat block of metal in a thickness range of 0.50 to 1.00 inches (12.7 to 25.4 mm).

A2.3.3.3 Adjust the instrument gain control(s) to produce an indication of 80 % of the upper linearity limit from the first back reflection signal from the block.

A2.3.3.4 Increase the external attenuator setting and the instrument gain control setting in 2 dB steps until the external attenuation is at 40 dB. At each step read and record the amplitude of the instrument display (or record output) indication.

A2.3.3.5 Further increase the external attenuation and instrument gain in 4 dB steps until a total of 80 dB attenuation and gain increase is obtained. (A lower maximum figure may be used if required by the instrument gain limitation.) At each step read and record the amplitude of the instrument display (or record output) indication.

A2.3.3.6 If the instrument indication is within ± 5 % of the original 80 % reading (76 % - 84 %) the gain control accuracy is suitable for distance-amplitude block checking by this procedure.

A2.4 Procedure

A2.4.1 *Adjustment of Sensitivity*—Using a search unit that meets the requirements of 11.5 set the water path length to its measured Y_0^+ value and normalize on the front surface of the reference block with a metal path of 0.500 inches (12.7 mm) or one with a metal path as near to this value as exists in the set to be checked. Set the instrument damping control (if provided) to its minimum value. Adjust the instrument gain so that the normalized front surface indication from the block is at 80% of the upper linearity limit (or as near to this value as can be obtained with the minimum gain control steps available). Adjust the instrument power control (if provided) to a value that will produce this indication amplitude with minimum instrument gain. Depending upon the size of the flat bottom holes in the blocks to be checked increase the instrument gain by the amount shown in Table A2.1.

A2.4.2 *Distance Amplitude Checking*—Using the gain and water path as determined in A2.4.1 carefully angulate the search unit to obtain the peak indication from the flat bottom hole in each block in the set and record these values. Blocks are acceptable if they meet the other requirements of this practice and if all indications fall within the limits specified in 11.8.2.

TABLE A2.1 Gain Increase for Distance-Amplitude Block Checking

Flat Bottom Hole Size	Gain Increase (dB)
#3	34
#5	25
#8	17

NOTE A2.1—With higher damping and lower power output than prescribed in A2.4.1 it may be possible, especially with ceramic transducers, to resolve peak indications from blocks with metal travel path lengths of less than 0.500 inches (12.7 mm). If these are included in a report, either the same damping and power output must be used for all blocks or a separate curve be provided showing overlap of the response amplitudes of the shorter metal path blocks with at least that from the 0.500 inch (12.7 mm) block examined under the same conditions.

APPENDIX

(Nonmandatory Information)

X1. RECOMMENDED TUNING NETWORK FOR LOW CAPACITANCE SEARCH UNITS

X1.1 *Circuit Configuration*⁶—A suggested design is shown in Fig. X1.1.

X1.2 *Component Values*—For a 5.0 MHz quartz crystal search unit as specified in 11.3.5, and assuming a total capacitance of 200 pF for search unit, cables, and manipulator, the following component values are recommended:

X1.2.1 L —5 μH tapped at $\frac{1}{3}$ from ground,

X1.2.2 C —1000 pF,

X1.2.3 C_T —Variable 50 pF, max,

X1.2.4 R_D —Variable 10 K Ω , max,

X1.2.5 R_1 —180 Ω , and

X1.2.6 R_2 —10 K Ω .

X1.3 *Component Ratings*—All components must have power and voltage ratings suitable for the applied pulser output.

⁶ Assembled networks may be obtained from specialty electronic services knowledgeable in ultrasonic pulser circuitry.

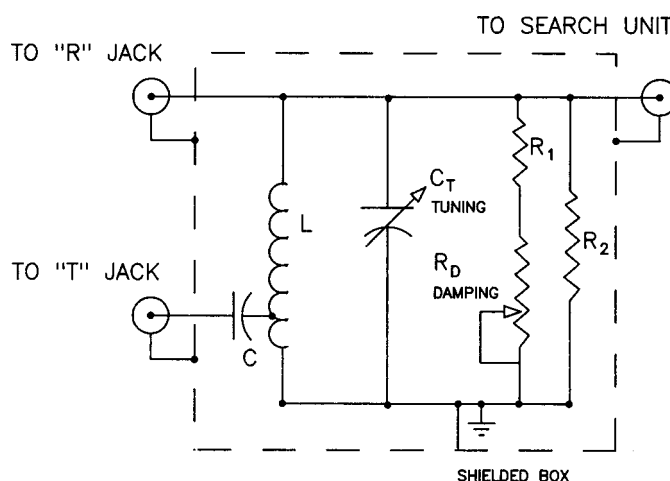


FIG. X1.1 Schematic Diagram for Tuning Network

X1.4 *Instrument Settings*—Operate in the “Through Transmission” mode, with any pulse-damping controls set for minimum (that is, maximum pulse-length). Adjust the network controls to obtain the test frequency and resolution required.

REFERENCES

- (1) Anon. (ASTM E07.06), “ASTM Research Report on E127 Annex,” ASTM Research Report RR:E07-1000.
- (2) Anon., “Ultrasonic Measurement Services,” *NIST Calibration Services Users Guide 1989*. Ed., J. Simmons, NIST Special Publication 250, 1989, pp 40–45.
- (3) Beck, K.H., “Limitations to the use of Reference Blocks for Periodic and Preinspection Calibration of Ultrasonic Inspection Instruments and Systems,” *Materials Evaluation*, Vol. 57, No.3, March 1999.
- (4) Blessing, G. V., “An Assessment of Ultrasonic Reference Block Calibration Methodology,” National Bureau of Standards Report NBSIR 83-2710, 1983.
- (5) Blessing, G. V., and Eitzen, D. G., “Variables affecting ultrasonic reference block calibration,” *1982 Paper Summaries*, ASNT National Spring Conference, March 22–25, 1982, Boston, MA, pp 287–291.
- (6) Blessing, G. V., and Eitzen, D. G., “Ultrasonic artifact calibration methodology,” *Office of Nondestructive Evaluation Technical Activities, 1985*. Edited by G. Birnbaum. National Bureau of Standards Report NBSIR 85-3187, 185.
- (7) Burley, C. E., “Calibration blocks for ultrasonic testing,” *Nondestructive Testing—A Review*, Edited by Harold Berger, ASTM, STP 624, 1977, pp 146–158.
- (8) Chwirut, D. J., “Recent Improvements to the ASTM-type Ultrasonic Reference Block System,” National Bureau of Standards Report, NBSIR 79-1742, 1979.
- (9) Chwirut, D. J., and Boswell, G. D., “The Evaluation of Search Units Used for Ultrasonic Reference Block Calibrations,” National Bureau of Standards Report NBSIR 78-1454, 1978.
- (10) Chwirut, D. J., Sushinsky, G. F., and Eitzen, D. G., “Procedures for the Calibration of ASTM E127—Type Ultrasonic Reference Blocks,” National Bureau of Standards Technical Note 924, Note 1976.
- (11) Cline, C. W., and Morgan, J. B., “Standardization in ultrasonic testing,” *Nondestructive Testing*, Vol 23, July–August, p 23.
- (12) Eitzen, D. G., et al., “Improved Ultrasonic Standard Reference Blocks,” National Bureau of Standards Report NBSIR 75-685, 1975.
- (13) Panian, F. C., and Van Valkenburg, H. E., “Development of ASTM Standard Reference Blocks for Ultrasonic Inspection,” *Proceedings, American Society for Testing and Materials*, Vol 59, 1959, pp 1237–1260.



- (14) Posakony, G. J., “Performance differences in quartz ultrasonic search units,” *Ultrasonic Materials Characterization*, H. Berger and M. Linzer, eds., Proceedings of the First International Symposium on Ultrasonic Materials Characterization, NBS, Gaithersburg, MD, June 7–9, 1978, National Bureau of Standards Special Publication 596, 1980, pp 595–603.
- (15) Slotwinski, J. A., and G. V. Blessing, “NIST Calibration of ASTM

E127–Type Ultrasonic Reference Blocks,” *NIST Report NISTIR 5430*, U.S. Dept. of Commerce Technology Administration, NIST, Gaithersburg, MD, May 1994.

- (16) Sushinsky, G. F., Eitzen, D. G., and Chwirut, D. J., “Improved Ultrasonic Standard Reference Blocks,” National Bureau of Standards Report NBSIR 76-984, 1976.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).