



Standard Test Methods for Measurement of Gloss of High-Gloss Surfaces by Abridged Goniophotometry¹

This standard is issued under the fixed designation E430; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 These test methods cover the measurement of the reflection characteristics responsible for the glossy appearance of high-gloss surfaces. Three test methods, A, B and C, are provided for evaluating such surface characteristics at specular angles of 30°, 20° and 30°, respectively. These test methods are not suitable for diffuse finish surfaces nor do they measure color, another appearance attribute.

1.2 As originally developed by Tingle and others (see Refs **1** and **2**),² the test methods were applied only to bright metals. Recently they have been applied to high-gloss automotive finishes and other nonmetallic surfaces.

1.3 The DOI of a glossy surface is generally independent of its curvature. The DOI measurement by this test method is limited to flat or flattenable surfaces.

2. Referenced Documents

2.1 ASTM Standards:³

D523 Test Method for Specular Gloss

D2457 Test Method for Specular Gloss of Plastic Films and Solid Plastics

E171 Specification for Atmospheres for Conditioning and Testing Flexible Barrier Materials

E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods

¹ These test methods are under the jurisdiction of ASTM Committee **E12** on Color and Appearance and are the direct responsibility of Subcommittee **E12.03** on Geometry.

Current edition approved June 1, 2011. Published June 2011. Originally approved in 1971. Last previous edition approved in 2005 as E430 – 05. DOI: 10.1520/E0430-11.

² The boldface numbers in parentheses refer to the list of references at the end of this method.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E179 Guide for Selection of Geometric Conditions for Measurement of Reflection and Transmission Properties of Materials

E284 Terminology of Appearance

E308 Practice for Computing the Colors of Objects by Using the CIE System

E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

E1347 Test Method for Color and Color-Difference Measurement by Tristimulus Colorimetry

3. Terminology

3.1 *Definitions*—Appearance terms in this test method are in accordance with Terminology **E284**.

3.2 Terms that are defined in Terminology **E284**, but have a specific definition in this method are:

3.2.1 *reflectance, p, n*—ratio of the reflected radiant or luminous flux to the incident flux in the given conditions. (**E284**)

3.2.1.1 *Discussion*—The term *reflectance* is often used in a general sense or as an abbreviation for *reflectance factor*. Such usage is not assumed in this method. The definition may require that the term be modified by adjectives denoting the spectral and geometric conditions of measurement.

3.3 *Definitions of Terms Specific to This Standard:*

3.3.1 *reflection haze, H, n*—for a specified specular angle, ratio of flux reflected at a specified angle (or angles) from the specular direction to the flux similarly reflected at the specular angle by a specified gloss standard.

3.3.1.1 *Discussion*—Modifiers may be used to specify the angles at which the haze is measured (for example, 2°, –5° or 15°); whether *–H* or a logarithmic form is to be stated; or whether *H* is to be compensated for the luminance of the specimen by multiplication by Y_{specimen}/Y_n , where *n* denotes the reference white; or any combination of these.

3.3.2 *metallic brightness, n*—freedom of a metal surface from diffuse haze or texture.

3.3.3 'with-machine' direction, n —the axis of a specimen that is parallel to the direction of mill rolling or extrusion, or other surface-finish texture.

3.3.4 'across-machine' direction, n —the perpendicular to 'with-machine' direction.

4. Summary of Test Method

4.1 Several geometrically different measures of light reflected by a surface are proposed for use in describing its gloss appearance.

4.1.1 *Test Method A*—A gloss reflectance factor is measured at 30° to the specimen normal using narrow illuminator and receiver aperture angles (0.5° wide maximum). Distinctness-of-image gloss is measured at 29.7° or 30.3° , or both. Narrow-angle (2°) reflection haze is measured at 28° or 32° , or both, and wide-angle (5°) reflection haze at 25° or 35° , or both. The ratio of reflectance factors for 28° or 32° , or both, perpendicular and parallel to the machine direction of the specimen, is computed as a measure of directionality.

4.1.2 *Test Method B*—A specular gloss is measured at 20° in accordance with Test Method D523, and narrow-angle reflection

haze is measured at 18.1° and 21.9° . For additional information on the selection of geometric conditions, see Guide E179.

4.1.3 *Test Method C*—A gloss reflectance factor is measured at 30° to the specimen normal using narrow illuminator and receiver aperture angles (0.5° wide maximum). Distinctness-of-image gloss is measured at 29.7° and 30.3° . Narrow-angle (2°) reflection haze is measured at 28° and 32° , and wide-angle (15°) reflection haze at 15° .

5. Significance and Use

5.1 The gloss of metallic finishes is important commercially on metals for automotive, architectural, and other uses where these metals undergo special finishing processes to produce the appearances desired. It is important for the end-products, which use such finished metals that parts placed together have the same glossy appearance.

5.2 It is also important that automotive finishes and other high-gloss nonmetallic surfaces possess the desired finished appearance. The present method identifies by measurements important aspects of finishes. Those having identical sets of

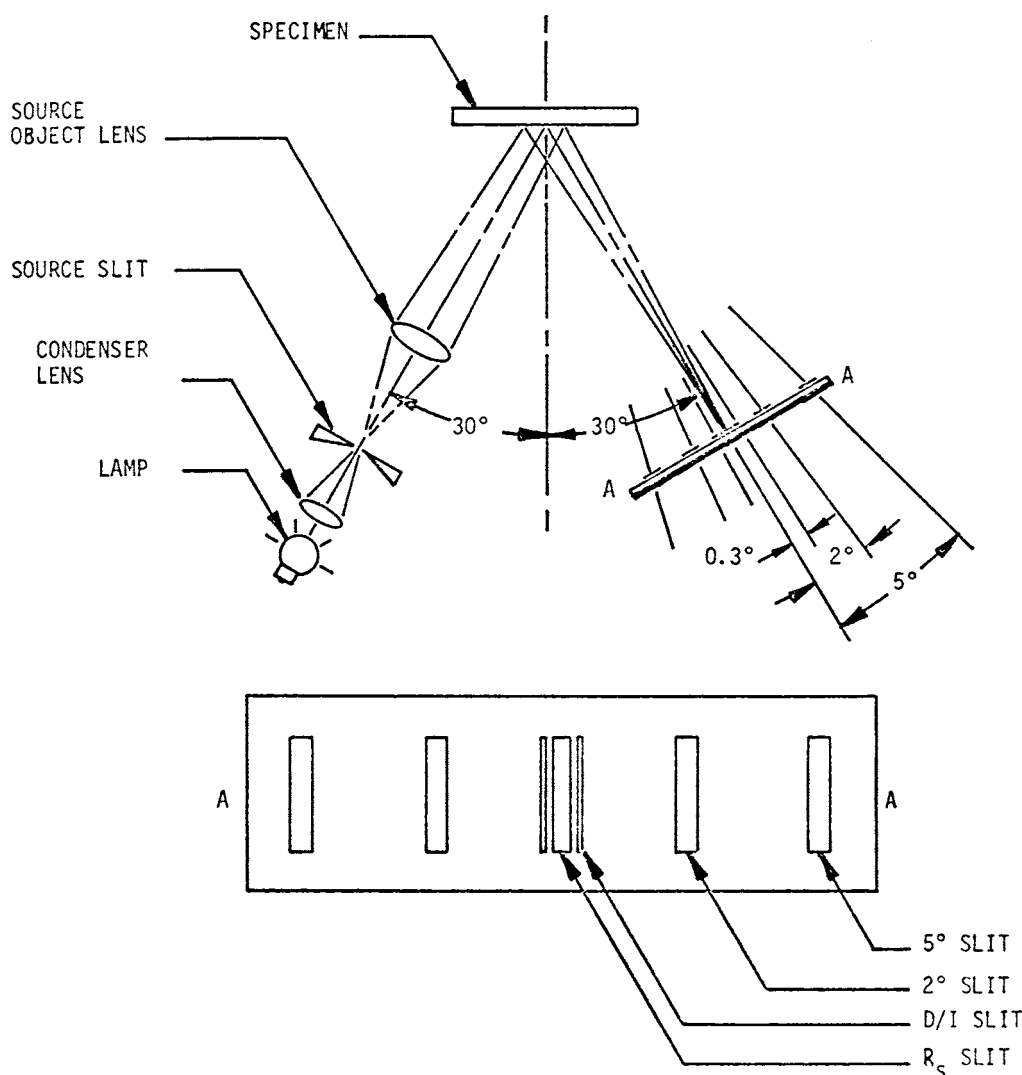


FIG. 1 Optical Diagram of the Apparatus for Method A

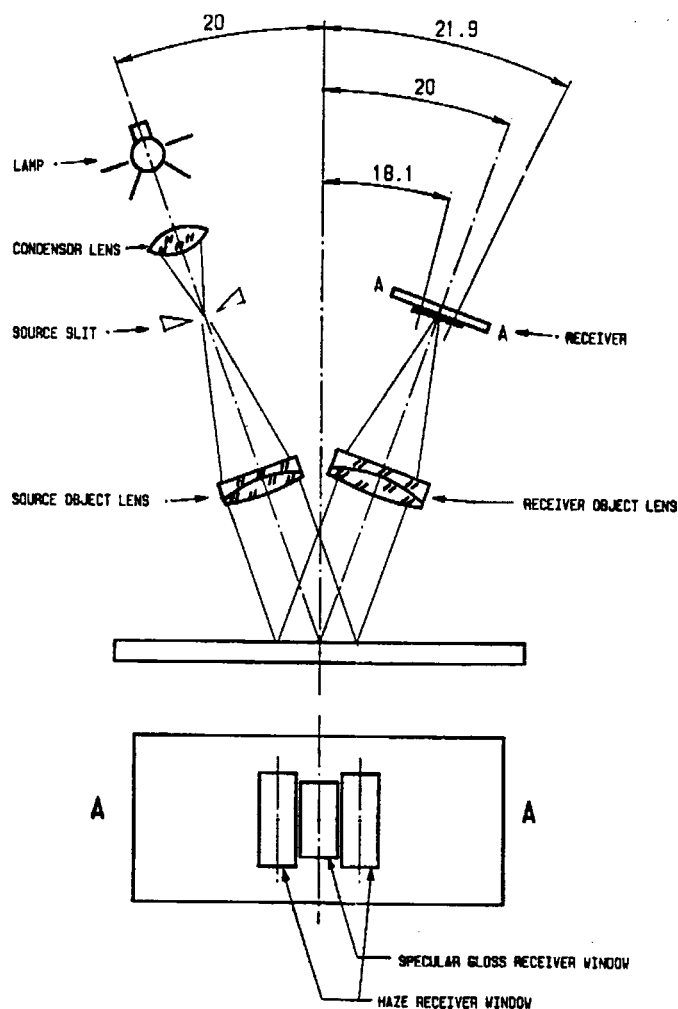


FIG. 2 Optical Diagram of the Apparatus for Method B

numbers normally have the same gloss characteristics. It usually requires more than one measurement to identify properly the glossy appearance of any finish (see Refs 3 and 4).

6. Apparatus

6.1 The apparatus shall be an abridged goniophotometer (see Fig. 1, Fig. 2, and Fig. 3). The abridged goniophotometer may have a fixed angle of incidence (for Test Method A, 30°; for Test Method B, 20°; for Test Method C, 30°) and specific fixed directions of view at which the flux from the specimen is measured (see Table 1, Table 2, and Table 3).⁴

6.1.1 *Geometric Conditions for Test Method A*—The direction of incidence shall be 30°. The directions of view shall be opposite the direction of incidence at 30° for specular reflectance, 29.7° or 30.3° for distinctness of image comparisons, 28° or 32° for narrow-angle haze comparisons, and 25° or 35° for wide-angle haze comparisons. The angular dimensions of

the mirror reflected image of the source slit in the plane of measurement and the angular dimensions of the receiver windows in this plane of measurement shall be as shown in Table 1.

6.1.2 *Geometric Conditions for Test Method B*—The direction of incidence shall be 20° ± 0.1°. The directions of view shall be opposite the direction of incidence, at 20° for specular gloss measurement and at 18.1° and 21.9° for narrow-angle reflection haze measurement. The angular dimensions of the specularly reflected image of the source slit in the plane of measurement and the angular dimensions of the receiver windows in this plane of measurement shall be as shown in Table 2.

6.1.3 *Geometric Conditions for Test Method C*—The direction of incidence shall be 30°. The directions of view shall be opposite the direction of incidence at 30° for specular reflectance, 29.7° and 30.3° for distinctness of image comparisons, 28° and 32° for narrow-angle haze comparisons, and 15° for wide-angle haze comparisons. The angular dimensions of the mirror reflected image of the source slit in the plane of measurement and the angular dimensions of the receiver windows in this plane of measurement shall be as shown in Table 3.

6.1.4 *Spectral Conditions*—The measurement shall be made with visible light to give results in accordance with the CIE spectral luminous efficiency function $V(\lambda)$, which is identical with $\bar{y}$ in the CIE 1931 standard observer and CIE standard illuminant C (see Practice E308 and Test Method E1347). If another illuminant such as A, is used, this shall be specified in the report.

6.1.5 *Polarization*—The incident flux shall be unpolarized and the receiver shall be insensitive to the state of polarization of the reflected luminous flux.

6.1.6 *Clamp*—For Test Method A, a rotatable clamp of the type shown in Fig. 4 may be used for flattening and positioning the specimen during measurement.

6.1.7 *Weights*—For Test Method C, a unit orientation or a weight similar to the type shown in Fig. 5 may be used for flattening and positioning the specimen during measurement.

7. Standards

7.1 Three calibrated standards of good planarity shall be available in either a set of metals or a set of nonmetals, depending upon which type of surface is measured.

7.2 High-Gloss Standards:

7.2.1 *High-Gloss Standard for Metals* shall be of aluminum, evaporated onto glass and covered with a protective coating of silicon monoxide, and calibrated for specular gloss and distinctness-of-image gloss.

7.2.2 *High-Gloss Standard for Nonmetals* shall be of highly polished black glass with a refractive index of approximately $n_D = 1.527$, calibrated for specular gloss and reflection haze, and assigned a scale value of $G_s = 89.4$ for a specular angle of 30° (Test Methods A and C) or $G_s = 89.2$ for a specular angle of 20° (Test Method B).

NOTE 1—To determine the scale value, calculate the first-surface (Fresnel) reflectance (see Test Method D2457, Instrumental Components in Apparatus section) for $n_D = 1.567$ and the specular angle of interest; for 30° it is 5.0436 % and for 20° it is 4.9078 %. Assign this a scale value of

⁴ The sole source of supply of the apparatus known to the committee at this time for Method A is Hunter Associates Laboratory, Reston, VA, for Method B is BYK-Gardner USA, Columbia, MD, and for Method C is TRICOR Systems Inc., Elgin, IL. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

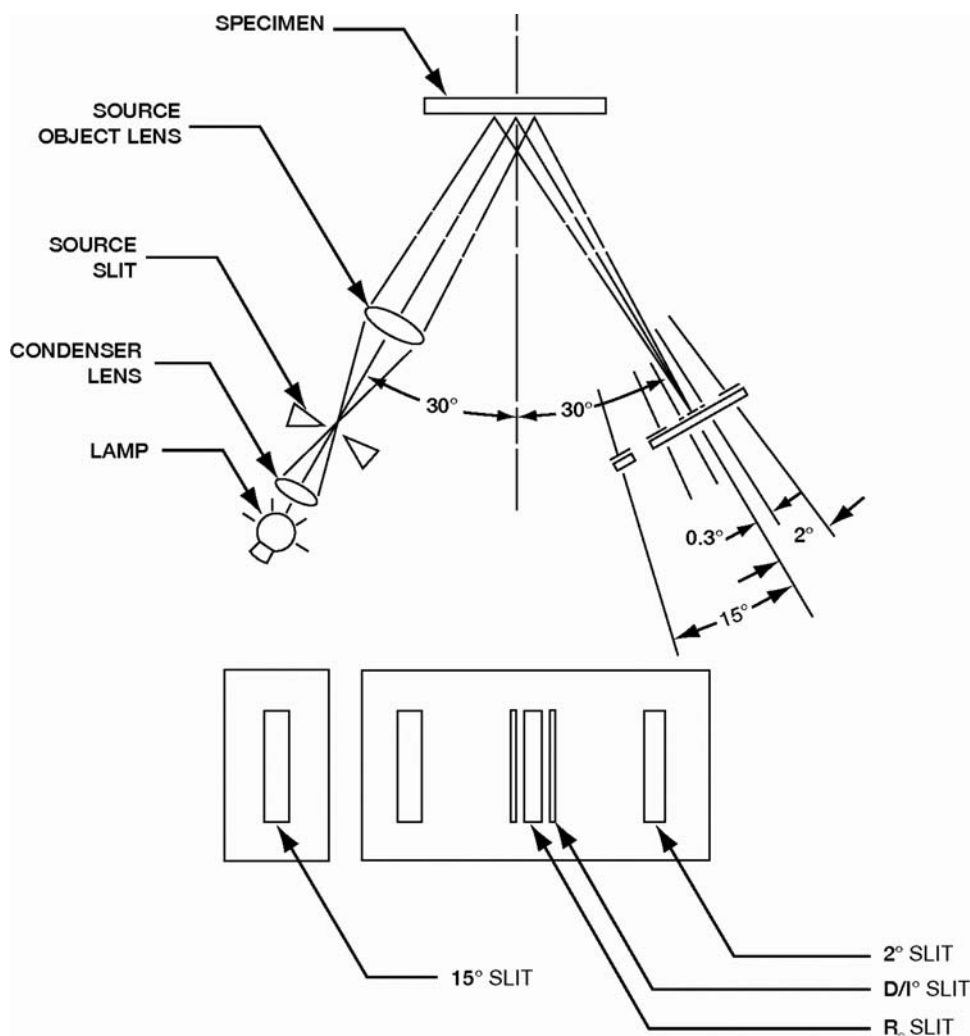


FIG. 3 Optical Diagram of the Apparatus for Method C

TABLE 1 Dimensions of the Mirror Image of the Source-Slit and of the Receptor Windows Measured in the Plane of the Receiving Windows (see Fig. 1)

Method A	Source-Slit Mirror Image, °	Specular Receiver Window, °	Distinctness-of-Image (± 0.29) Receiver Window, °	Haze Receiver Windows, °
Angle of center of window (measured from perpendicular to specimen surface)	30	30	30.3 and 29.7	28 and 32 or 25 and 35
Width (in the plane of the angle of reflection)	0.44 ± 0.01	0.4 ± 0.01	0.14 ± 0.01	0.4 ± 0.1 or 0.5 ± 0.1
Length (across the plane of the angle of reflection)	5.0 ± 1	3.0 ± 1	3.0 ± 1	3.0 ± 1

100 (see Test Method D523, Primary Standards in Reference Standards section). Repeat the calculation for $n_p = 1.527$ and the same specular angle; the result for 30° is 4.5069 % and for 20° , 4.3769 %. The new scale value for 30° is $100 \times (4.5069/5.0436) = 89.4$, and for 20° , $100 \times (4.3769/4.9078) = 89.2$. (The latter value is also given in Test Method D523.)

7.3 Intermediate Standards:

7.3.1 *Intermediate Standard for Metals* shall be of either chromium evaporated onto glass and covered with a protective

coating of silicon monoxide, or of bright sheet aluminum with protective coating and calibrated for specular gloss and distinctness-of-image gloss.

7.3.2 *Intermediate Standard for Nonmetals* shall be of a ceramic material, such as porcelain enamel on steel, and calibrated for specular gloss and distinctness-of-image gloss.

7.4 *Diffuse Standards* shall have a reflectance factor substantially constant over the angular range of the instrument.

TABLE 2 Dimensions of the Specular Image of the Source-Slit and of the Receptor Windows Measured in the Plane of the Receiving Windows (see Fig. 2)

Method B	Source-Slit Specular Image, °	Specular Gloss Receiver Window, °	Haze Receiver Window, °
Angle of center of window (measured from perpendicular to specimen surface)	20.0 ± 0.1	20.0 ± 0.1	18.1 ± 0.1 and 21.9 ± 0.1
Width (in the plane of the angle of reflection)	0.75 ± 0.1	1.8 ± 0.05	1.8 ± 0.1
Length (across the plane of the angle of reflection)	2.5 ± 0.25	3.6 ± 0.1	5.5 ± 0.25

TABLE 3 Dimensions of the Mirror Image of the Source-Slit and of the Receptor Windows Measured in the Plane of the Receiving Windows (see Fig. 3)

Method C	Source-Slit Mirror Image, °	Specular Receiver Window, °	Distinctness-of-Image (±0.29) Receiver Window, °	Haze Receiver Windows, °
Angle of center of window (measured from perpendicular to specimen surface)	30	30	30.3 and 29.7	28 and 32 (2° Haze) 15 (15° Haze)
Width (in the plane of the angle of reflection)	0.44 ± 0.01	0.4 ± 0.01	0.14 ± 0.01	0.4 ± 0.1 (2° Haze) 1.91 ± 0.1 (15° Haze)
Length (across the plane of the angle of reflection)	5.0 ± 1	0.62 ± .01	0.62 ± .01	0.62 ± .01 (2° Haze) 0.62 ± .01 (15° Haze)

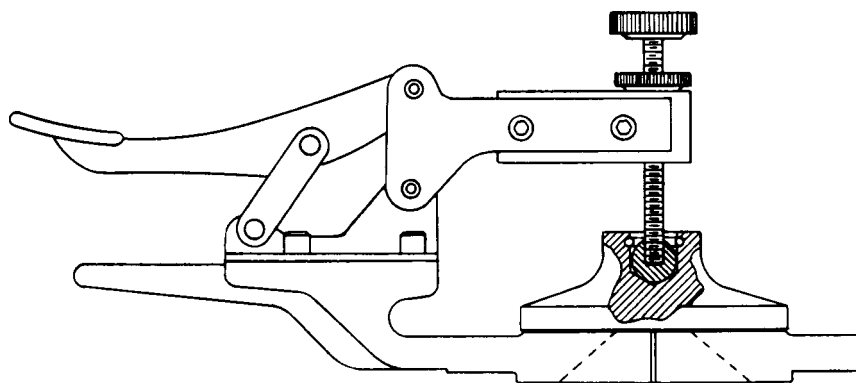


FIG. 4 A Rotatable Clamp Suggested for Flattening the Specimen and Positioning It During Measurement (Method B)

7.5 Care of Standards—It is essential that the standards be kept clean and free of scratches as well as from contact with contaminating materials. The cleaning method specified by the instrument manufacturer shall be followed and the standards should be checked at regular intervals against reference standards held in reserve.

8. Specimens

8.1 Specimens shall be obtained from test samples by selecting areas that are plane and representative of each sample being tested. Every specimen must be at least 2¾ in. (70 mm) in the smallest dimension. Specimens may be larger so long as it is possible to insert them into the instrument and flatten them properly for measurement.

8.2 For Method A, a specimen may be considered to be properly flattened when no portion of the measured specimen surface deviates from the sample plane by more than 0.15 deg.

9. Preparation and Standardization of Apparatus

9.1 The instrument must be used in a clean dry area free of drafts. Standard laboratory conditions are recommended (see

Referenced Documents section in Specification E171). Voltage regulation to ±0.01 % must be incorporated in the instrument, or supplied separately. Follow manufacturer's recommendations for instrument warm-up.

9.2 **Standardization**—Adjust the instrument to read the same gloss reflectance factor for the intensity of light reflected from the diffuse standard through the specular, distinctness-of-image, and haze apertures. Adjust the instrument to read values of specular gloss and distinctness-of-image gloss assigned the aluminum mirror if metal surfaces are being measured; or the black gloss standard if nonmetal surfaces are being measured. If the instrument does not then read the appropriate intermediate standard within the limits set by the instrument manufacturer, refocus or restandardize following the manufacturer's instructions.

10. Procedure

10.1 Bring the specimen to the instrument for measurement. Be sure the specimen is flat.

NOTE 2—The measured DOI will be erroneously low in the measurement direction if there is excessive specimen curvature in that direction.

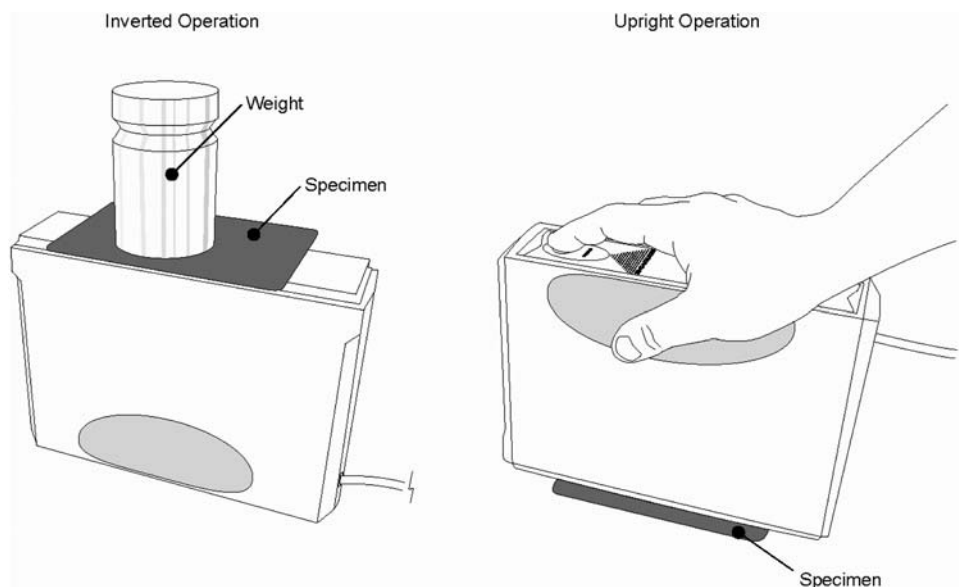


FIG. 5 Suggested Methods for Maintaining or Flattening Specimen During Measurement (Method C)

10.2 For Test Method A and C, be certain that the specular sensor is centered on the specimen-reflected specular light beam. The full goniophotometer, shown in Fig. 6, identifies the specular direction by the peak of the goniophotometric curve.

10.3 Rotate the specimen in its own plane to find the orientation, giving the maximum specular signal. This specimen orientation is called the “machine direction” because it generally coincides with the direction of travel of a sheet or film material through a processing machine.

10.4 Record the following quantities:

10.4.1 For Test Method A, readings of (a) gloss reflectance factor (specular gloss), $R_{s,30}$ at 30° ; (b) distinctness-of-image gloss; (c) 2° reflection haze; H_2 ; and (d) 5° reflection haze, H_5 . The quantities in (b), (c), and (d) may be either gloss reflectance factors or values of H , which are their ratios to the specular gloss reflectance factor recorded in (a).

10.4.2 For Test Method B, readings of (a) the 20° specular gloss, $R_{s,20}$; (b) the reflection haze, H ; and (c) the luminous reflectance, Y .

10.4.3 For Test Method C, readings of (a) gloss reflectance factor (specular gloss), $R_{s,30}$ at 30° ; (b) distinctness-of-image gloss; (c) 2° reflection haze; H_2 ; and (d) 15° reflection haze, H_{15} . The quantities in (b), (c), and (d) may be either gloss reflectance factors or values of H , which are their ratios to the specular gloss reflectance factor recorded in (a).

10.5 Measure at least three areas of each specimen.

10.6 From these same areas, read 2° haze for the “across-machine direction,” being careful to flatten the test surface and orient the specular beam in each case.

10.7 Take readings on the standards at the end of the series of observations to ensure that the instrument has remained in calibration throughout the operation.

NOTE 3—Poor measurement repeatability may be due to failures to sufficiently flatten the specimen.

11. Calculation

11.1 For Test Method A, calculate the mean of three readings for each specimen for:

11.1.1 Specular gloss, $R_{s,30}$, at 30° .

11.1.2 Distinctness-of-image gloss, $100 \times (1 - H_{0.3})$, evaluated at 0.3° on either or both sides of the specular angle.

11.1.3 2° Reflection haze, $100 H_2$, evaluated at 2° on either or both sides of the specular angle.

11.1.4 5° Reflection haze, $100 H_5$, evaluated at 5° on either or both sides of the specular angle.

11.1.5 Directionality, $100 \times (H_{2, \text{across-machine}}/H_{2, \text{with-machine}})$, evaluated at 2° on either or both sides of the specular angle.

11.2 For Test Method B, calculate the mean of three readings of each specimen for:

11.2.1 Specular gloss, $R_{s,20}$ at 20° .

11.2.2 One or more of the following, as required:

11.2.2.1 Reflection haze, H_{20} .

11.2.2.2 Logarithmic reflection haze, $H_{20,\log} = 1285 \log[(H_{20}/20) + 1]$.

11.2.2.3 Compensated reflection haze, $H_{20,\text{comp}} = H_{20, \text{specimen}} - (H_{20,n} \times Y_{\text{specimen}}/Y_n)$.

NOTE 4— $H_{20,\log}$ may also be calculated as a compensated quantity by using $H_{20,\text{comp}}$ in place of H_{20} in 11.2.2.2. Compensated quantities shall be used when comparing specimens with different values of Y .

11.3 For Test Method C, calculate the mean of three readings for each specimen for:

11.3.1 Specular gloss, $R_{s,30}$, at 30° .

11.3.2 Distinctness-of-image gloss, $100 \times (1 - H_{0.3})$, evaluated at 0.3° on both sides of the specular angle.

11.3.3 2° Reflection haze, $100 H_2$, evaluated at 2° on either or both sides of the specular angle.

11.3.4 15° Reflection haze, $100 H_{15}$, evaluated at 15° from the specular angle.

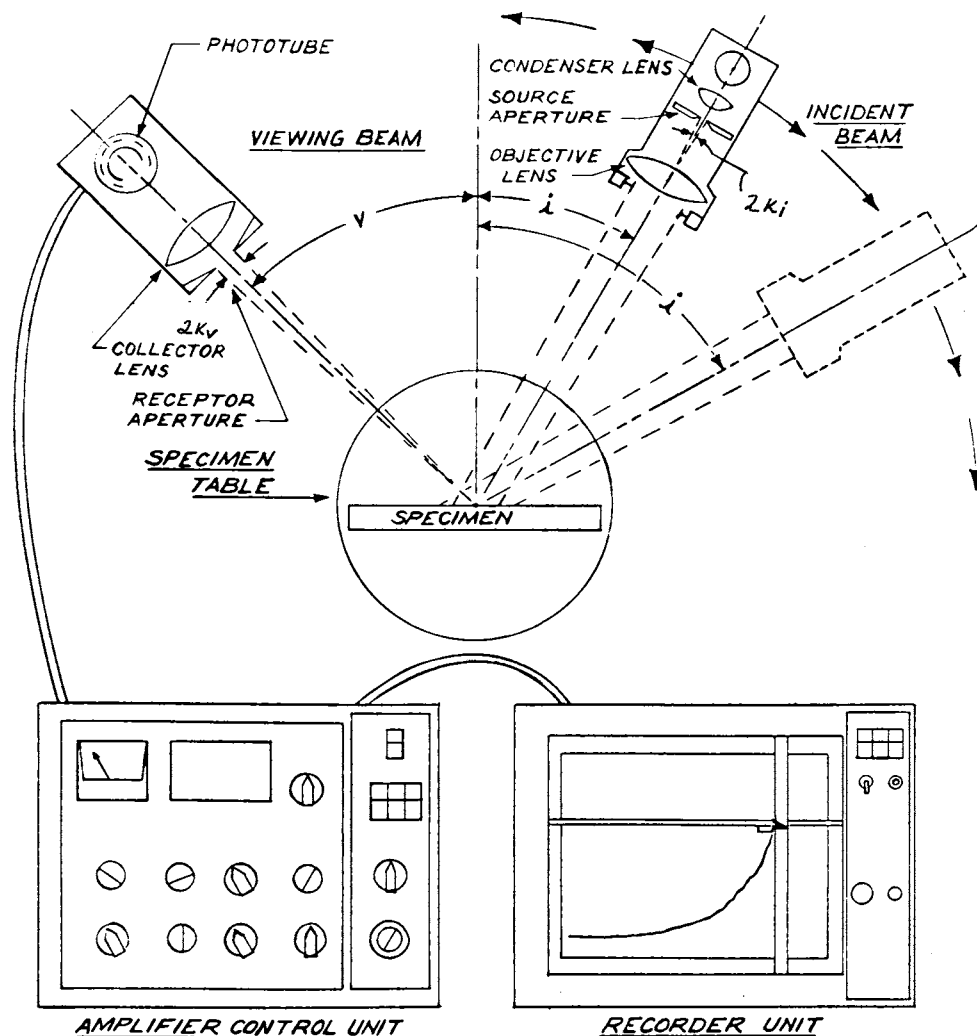


FIG. 6 Recording Goniophotometer Showing Viewing Angle, v , Incidence Angle, i , and Their Respective Field Angles, $2K_v$ and $2K_i$

11.3.5 Directionality, $100 \times (H_{2, \text{ across-machine}}/H_{2, \text{ with-machine}})$, evaluated at 2° on both sides of the specular angle.

12. Report

12.1 The report for Test Method A shall contain the following:

- 12.1.1 The specular gloss $R_{s,30}$,
- 12.1.2 The distinctness-of-image gloss,
- 12.1.3 The 2° haze, H_2 ,
- 12.1.4 The 5° reflection haze, H_5 ,
- 12.1.5 The directionality.

12.2 The report for Test Method B shall contain the following:

- 12.2.1 The specular gloss $R_{s,20}$,
- 12.2.2 Either the logarithmic reflection haze or the compensated logarithmic reflection haze.

12.3 The report for Test Method C shall contain the following:

- 12.3.1 The specular gloss $R_{s,30}$,
- 12.3.2 The distinctness-of-image gloss,
- 12.3.3 The 2° haze, H_2 ,
- 12.3.4 The 15° reflection haze, H_{15} .

12.4 The report for all methods shall contain the following:

- 12.4.1 Identification of instrument used by model and serial number,
- 12.4.2 Identification of gloss standards by number and scale value assigned,
- 12.4.3 Identification of any specimens whose values on any scale differ by more than 3.0 in individual readings from the averages reported, and
- 12.4.4 Identification of Test Method used (A, B, or C.)

13. Precision and Bias

13.1 Test Method A:

13.1.1 The precision of this test method is based on an inter-laboratory study of Method A of ASTM E430, Test Methods for Measurement of Gloss of High-Gloss Surfaces by Abridged Goniophotometry, conducted in 2007. Results in this study were obtained from two laboratories, testing seven coated panels. (Table 4) Every "test result" reported represents an individual determination. Both participating laboratories reported two replicate test results for each material. Except for the use of only two laboratories, Practice E691 was followed

TABLE 4 Distinctness of Image

Panel	Average ^A	Sample Standard Deviation	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
	$\bar{x}$	$s_{\bar{x}}$	s_r	s_R	r	R
1	98.425	0.601	0.250	0.626	0.700	1.754
2	98.700	0.566	0.000	0.566	0.000	1.584
3	98.625	0.813	0.150	0.820	0.420	2.296
4	97.975	0.672	0.320	0.709	0.896	1.985
5	98.000	1.131	0.100	1.134	0.280	3.174
6	94.275	0.884	0.650	0.996	1.820	2.789
7	97.275	0.955	0.602	1.045	1.686	2.927

^A The average of the laboratories' calculated averages.

for the design and analysis of the data; the details are given in ASTM Research Report No. E12-1006.⁵

13.1.2 Repeatability Limit (r)—Two test results obtained within one laboratory shall be judged not equivalent if they differ by more than the “ r ” value for that material; “ r ” is the interval representing the critical difference between two test results for the same material, obtained by the same operator using the same equipment on the same day in the same laboratory. (Table 5)

TABLE 5 Correlation with Visual Evaluation

Panel	Average ^A (instrumental)	Average (visual)	Correlation
	$\bar{x}_i$	$\bar{x}_v$	cc
1	98.425	7.92	
2	98.700	0	
3	98.625	5.77	
4	97.975	10	-0.8301

^A The average of the laboratories' calculated averages.

13.1.3 Reproducibility Limit (R)—Two test results shall be judged not equivalent if they differ by more than the “ R ” value for that material; “ R ” is the interval representing the critical difference between two test results for the same material, obtained by different operators using different equipment in different laboratories. (Table 6)

TABLE 6 Correlation with Visual Evaluation

Panel	Average ^A (instrumental)	Average (visual)	Correlation
	$\bar{x}_i$	$\bar{x}_v$	cc
1	98.000	2.3	
2	94.275	10	
3	97.275	6.47	
4	98.700	0	-0.9391

^A The average of the laboratories' calculated averages.

13.1.4 The above terms (repeatability limit and reproducibility limit) are used as specified in Practice E177.

13.1.5 Any judgment in accordance with statements 13.1.2 and 13.1.3 would normally have an approximate 95 % probability of being correct, however the precision statistics obtained in this ILS must not be treated as exact mathematical quantities which are applicable to all circumstances and uses.

⁵ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:E12-1006.

The limited number of laboratories representing results guarantees that there will be times when differences greater than predicted by the ILS results will arise, sometimes with considerably greater or smaller frequency than the 95 % probability limit would imply. The repeatability limit and the reproducibility limit should be considered as general guides, and the associated probability of 95 % as only a rough indicator of what can be expected.

13.1.6 Bias—At the time of the study, there was no accepted reference material suitable for determining the bias for this test method, therefore no statement on bias is being made.

13.1.7 The precision statement was determined through statistical examination of 28 results, from two laboratories, on seven panels. These seven panels were identified as the following:

- Panel 1: #B401 Black panel
- Panel 2: #B323 Black panel
- Panel 3: #B269 Black panel
- Panel 4: #B534 Black panel
- Panel 5: #G164 Metallic Green panel
- Panel 6: #S665 Metallic Silver panel
- Panel 7: #W915 White panel

To judge the equivalency of two test results, it is recommended to choose the panel closest in characteristics to the test panel.

13.2 Test Method B:

13.2.1 Precision—The repeatability standard deviation of Test Method B for 20° gloss is strongly dependent on the reported value of the log reflection haze. The black glass #638118, exhibited a log reflection haze of 0.055, and a repeatability standard deviation for 20° gloss of 0.045. Under these conditions, two measurements that differ by more than 0.126 should be considered suspect. For a tan-colored enamel plaque, whose log reflection haze was measured as 1.304, the repeatability standard deviation for 20° gloss was 0.321. Under these conditions, two measurements that differ by more than 0.90 should be considered suspect. These readings are uncompensated values of the reflection haze and as the compensation requires an additional measurement, the standard deviations and range of acceptable values will be different from the values given here.

13.2.2 The reproducibility of this method is being determined and will be available on or before January 15, 2012.

13.3 Bias—No information can be presented for the procedure for Methods A or B in Test Methods E430 because no material having an accepted reference value is available.

TABLE 7 Distinctness of Image

Panel	Average ^A $\bar{x}$	Sample Standard Deviation $s_{\bar{x}}$	Repeatability Standard Deviation s_r	Reproducibility Standard Deviation S_R	Repeatability Limit r	Reproducibility Limit R
1	90.200	3.182	0.930	3.249	2.604	9.098
2	96.650	2.333	1.005	2.439	2.814	6.830
3	91.700	3.748	0.604	3.772	1.692	10.561
4	83.600	5.091	0.781	5.121	2.187	14.339
5	94.650	2.687	0.652	2.726	1.825	7.634
6	83.400	4.384	1.000	4.441	2.800	12.434
7	85.450	5.233	0.474	5.243	1.328	14.681

^A The average of the laboratories' calculated averages.

13.4 Test Method C:

13.4.1 The precision of this test method is based on an inter-laboratory study of Method C of ASTM E430, Test Methods for Measurement of High-Gloss Surfaces by Abridged Goniophotometry, conducted in 2007. Results in this study were obtained from two laboratories, testing seven coated panels. (Table 7) Every “test result” reported represents an individual determination. Both participating laboratories reported two replicate test results for each material. Except for the use of only two laboratories, Practice E691 was followed for the design and analysis of the data; the details are given in ASTM Research Report No. E12–1006.⁵

13.4.2 *Repeatability Limit (r)*—Two test results obtained within one laboratory shall be judged not equivalent if they differ by more than the “*r*” value for that material; “*r*” is the interval representing the critical difference between two test results for the same material, obtained by the same operator using the same equipment on the same day in the same laboratory. (Table 8)

TABLE 8 Correlation with Visual Evaluation

Panel	Average ^A (instrumental) $\bar{x}_i$	Average (visual) $\bar{x}_v$	Correlation cc
1	90.200	7.92	
2	96.650	0	
3	91.700	5.77	
4	83.600	10	-0.9387

^A The average of the laboratories' calculated averages.

13.4.3 *Reproducibility Limit (R)*—Two test results shall be judged not equivalent if they differ by more than the “*R*” value for that material; “*R*” is the interval representing the critical difference between two test results for the same material, obtained by different operators using different equipment in different laboratories. (Table 9)

13.4.4 The above terms (repeatability and reproducibility limit) are used as specified in Practice E177.

13.4.5 Any judgment in accordance with statements 13.4.2 and 13.4.3 would normally have an approximate 95 % probability of being correct, however the precision statistics ob-

TABLE 9 Correlation with Visual Evaluation

Panel	Average ^A (instrumental) $\bar{x}_i$	Average (visual) $\bar{x}_v$	Correlation cc
5	94.650	2.3	
6	83.400	10	
7	85.450	6.47	
2	96.650	0	-0.9747

^A The average of the laboratories' calculated averages.

tained in this ILS must not be treated as exact mathematical quantities which are applicable to all circumstances and uses. The limited number of laboratories reporting results guarantees that there will be times when differences greater than predicted by the ILS results will arise, sometimes with considerably greater or smaller frequency than the 95 % probability limit would imply. The repeatability limit and the reproducibility limit should be considered as general guides, and the associated probability of 95 % as only a rough indicator of what can be expected.

13.4.6 *Bias*—At the time of the study, there was no accepted reference material suitable for determining the bias for this test method, therefore not statement on bias is being made.

13.4.7 The precision statement was determined through statistical examination of 28 results, from two laboratories, on seven panels. These seven panels were identified as the following:

- Panel 1: #B401 Black panel
- Panel 2: #B323 Black panel
- Panel 3: #B269 Black panel
- Panel 4: #B534 Black panel
- Panel 5: #G164 Metallic Green panel
- Panel 6: #S665 Metallic Silver panel
- Panel 7: #W915 White panel

To judge the equivalency of two test results, it is recommended to choose the panel closest in characteristics to the test panel.

14. Keywords

14.1 distinctness of image; goniophotometry; reflection characteristics; reflection haze; sheen; specular gloss

REFERENCES

- (1) Tingle, W. H., and Potter, F. R., “New Instrument Grades for Polished Metal Surfaces,” *Prod Eng*, Vol. 27, March 1961.
- (2) Tingle, W. H., and George, D. J., “Measuring Appearance Characteristics of Anodized Aluminum Automotive Trim,” Report No. 650513, Society of Automotive Engineers, May 1965.
- (3) Hunter, R. S., “Gloss Evaluation of Materials,” *ASTM Bulletin 186*, Am. Soc. Testing Mater., 1952.
- (4) Christie, J. S., “Instruments for Metallic Appearance,” *Appearance of Metallic Materials, ASTM STP 478*, Am. Soc. Testing Mater., 1970, pp. 59–78.
- (5) Christie, J. S., “An Instrument for the Geometric Attributes of Metallic Appearance,” *App Opt*, Vol. 8:1777–1785 (1969).

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).